

Annex F2

Surface Water Quality Monitoring Results

Table F2.1 Surface Water Quality Monitoring Results at DP4T

Date	Time	Weather Condition	Water Appearance	Water Condition	Water Temperature (°C)	Dissolved Oxygen (DO) (mg/L)	pH	Suspended Solids (SS) (mg/L)	Remarks
6 Feb 20	14:13	Sunny		Unable to collect water sample due to insufficient flow					-
12 Feb 20	14:23	Sunny		Unable to collect water sample due to insufficient flow					-
20 Feb 20	14:06	Sunny	Colourless	Semi-clear	17.7	9.83	7.91	18.6	-
20 Feb 20	14:06	Sunny	Colourless	Semi-clear	17.9	9.80	7.60	20.7	DP4 (Future, temporary) (Duplicate)
27 Feb 20	14:22	Sunny		Unable to collect water sample due to insufficient flow					-
					Average	9.82	7.76	19.7	-
					Min	9.80	7.60	18.6	-
					Max	9.83	7.91	20.7	-

Notes: DP4 was temporary relocated to DP4 (Future, temporary) (i.e. DP4T) as an interim discharge point from the monitoring event on 16 May 2019.

Table F2.2 Surface Water Quality Monitoring Results at DP6

Date	Time	Weather Condition	Water Appearance	Water Condition	Water Temperature (°C)	Dissolved Oxygen (DO) (mg/L)	pH	Suspended Solids (SS) (mg/L)
6 Feb 20	14:06	Sunny		Unable to collect water sample due to insufficient flow				
12 Feb 20	14:12	Sunny		Unable to collect water sample due to insufficient flow				
20 Feb 20	14:01	Sunny		Unable to collect water sample due to insufficient flow				
27 Feb 20	14:10	Sunny		Unable to collect water sample due to insufficient flow				
					Average	-	-	-
					Min	-	-	-
					Max	-	-	-

Figure F2.1 Graphical Presentation for Surface Water Quality Monitoring (DO)

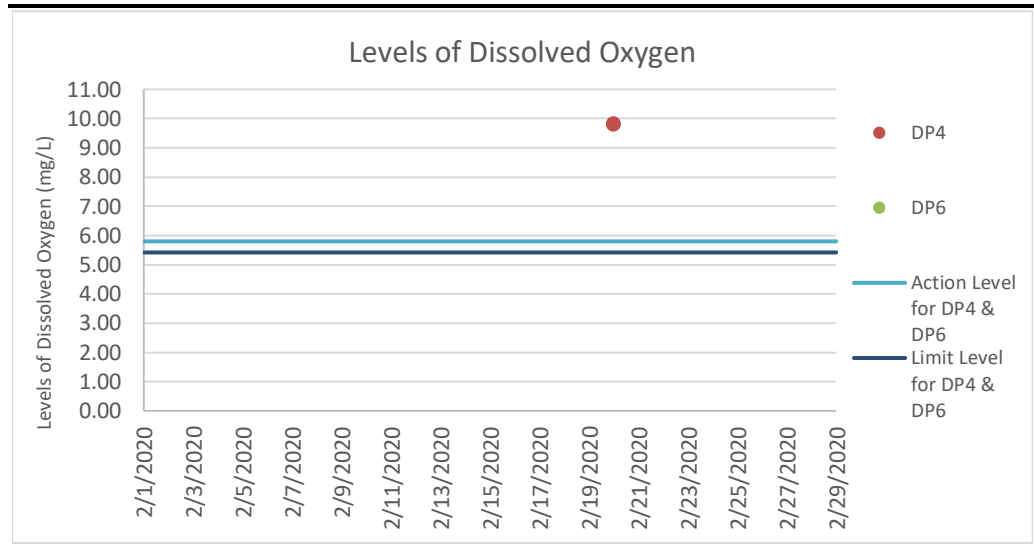


Figure F2.2 Graphical Presentation for Surface Water Quality Monitoring (pH)

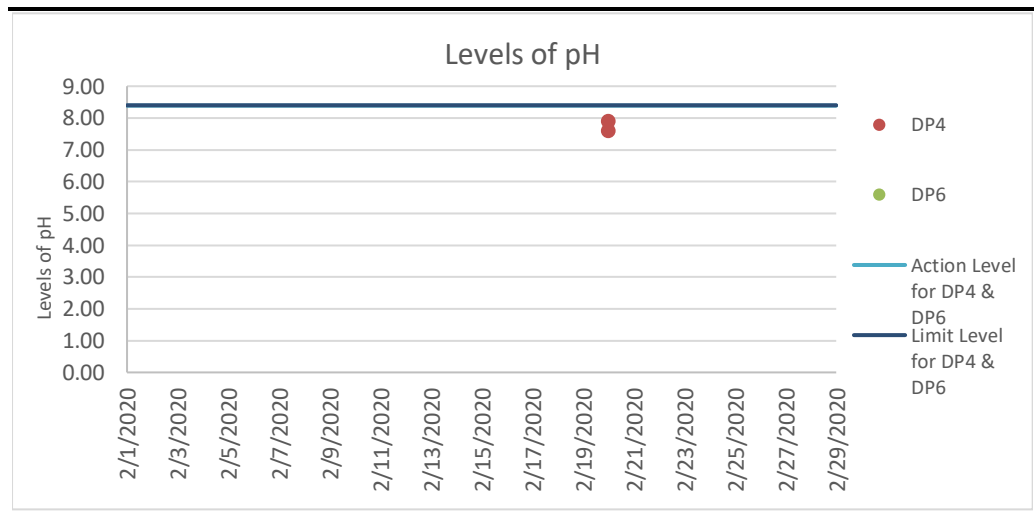


Figure F2.3 Graphical Presentation for Surface Water Quality Monitoring (SS)

