

Table F2.1 Surface Water Quality Monitoring Results at DP4T

Date	Time	Weather Condition	Water Appearance	Water Condition	Water Temperature (°C)	Dissolved Oxygen (DO) (mg/L)	pH	Suspended Solids (SS) (mg/L)	Remarks	
7 May 20	14:24	Sunny		Unable to collect water sample due to insufficient flow						-
14 May 20	14:18	Sunny		Unable to collect water sample due to insufficient flow						-
20 May 20	14:24	Cloudy		Unable to collect water sample due to insufficient flow						-
28 May 20	15:13	Rainy	Light yellow	Semi-clear	27.6	7.81	7.78	42.2	-	
						Average	7.81	7.78	42.2	-
						Min	7.81	7.78	42.2	-
						Max	7.81	7.78	42.2	-

Notes: DP4 was temporary relocated to DP4 (Future, temporary) (i.e. DP4T) as an interim discharge point from the monitoring event on 16 May 2019.

Table F2.2 Surface Water Quality Monitoring Results at DP6

Date	Time	Weather Condition	Water Appearance	Water Condition	Water Temperature (°C)	Dissolved Oxygen (DO) (mg/L)	pH	Suspended Solids (SS) (mg/L)	Remarks	
7 May 20	14:12	Sunny		Unable to collect water sample due to insufficient flow						-
14 May 20	14:03	Sunny		Unable to collect water sample due to insufficient flow						-
20 May 20	14:12	Cloudy	Colourless	Clear	27.2	8.01	8.21	6.1	-	
20 May 20	14:16	Cloudy	Colourless	Clear	27.2	8.01	8.25	6.2	DP6 (Duplicate)	
28 May 20	14:48	Rainy	Light yellow	Semi-clear	27.7	7.50	7.32	17.7	-	
28 May 20	14:57	Rainy	Light yellow	Semi-clear	27.7	7.43	7.12	16.4	DP6 (Duplicate)	
						Average	7.74	7.73	11.6	-
						Min	7.43	7.12	6.1	-
						Max	8.01	8.25	17.7	-

Figure F2.1 Graphical Presentation for Surface Water Quality Monitoring (DO)

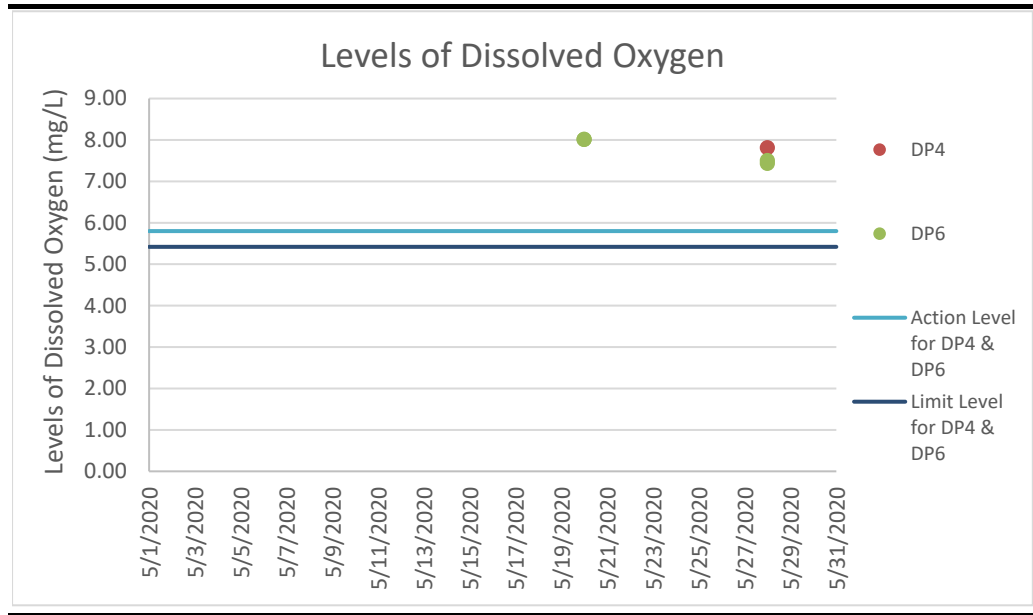


Figure F2.2 Graphical Presentation for Surface Water Quality Monitoring (pH)

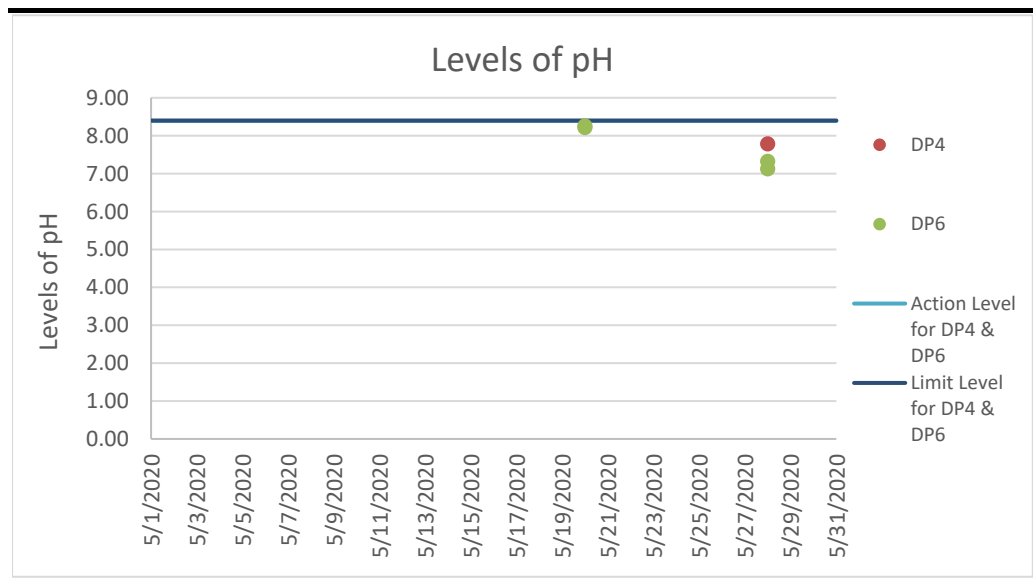


Figure F2.3 Graphical Presentation for Surface Water Quality Monitoring (SS)

