



Calibration Report of High Volume Air Sampler


Manufacturer : Graseby 105 **Date of Calibration** : 02 December 2020

Serial No. : 9795 (ET / EA / 003 / 18) **Calibration Due Date** : 01 February 2021

Method : Five-point calibration by using standard calibration kit Tisch TE-5025A refer to the Operations Manual

Results	Flow recorder reading (cfm)	49	45	40	32	28
	Qstd (Actual flow rate, m ³ /min)	1.73	1.52	1.26	1.05	0.85
	Pressure : 765.06 mm Hg	Temp. : 293 K				

Sampler 9795 Calibration Curve
Site: Tseung Kwan O 137 (TKO-A1)

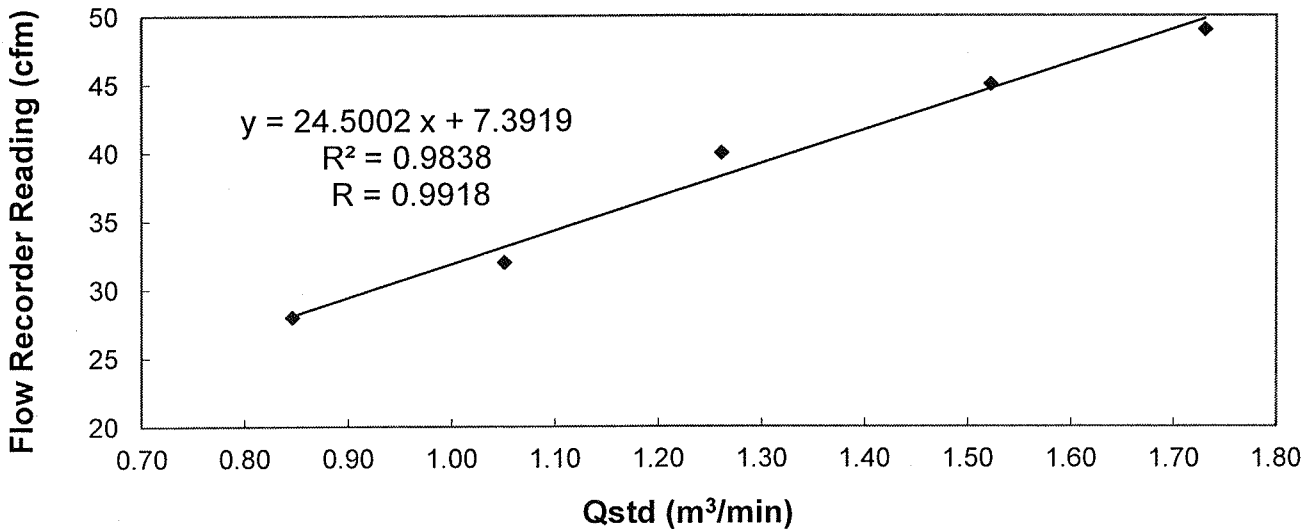

Acceptance Criteria : Correlation coefficient (r) of the calibration curve greater than 0.990 after a 5-point calibration

The high volume sampler complies* / ~~does not comply~~* with the specified requirements and is deemed acceptable*/ unacceptable* for use.

Calibrated by : *Man*
CHAN, Wai Man
(Technician)

Checked by : *[Signature]*
LAU, Chi Leung
(Environmental Team Leader)