

Annex D1

Calibration Certificates for Dust Monitoring Equipment

TSP SAMPLER CALIBRATION CALCULATION SPREADSHEET

Location ID : AM1	Date of Calibration: 19-May-22
Name and Model: TISCH HVS Model TE-5170	Next Calibration Date: 19-Jul-22
	Operator: Dixon Chan

CONDITIONS

Sea Level Pressure (hPa)	1011.9	Corrected Pressure (mm Hg)	758.925
Temperature (°C)	25.8	Temperature (K)	299

CALIBRATION ORIFICE

Make-> TISCH	Qstd Slope -> 1.99838
Model-> 5025A	Qstd Intercept -> -0.00903
Serial # -> 1612	

CALIBRATION

Plate No.	H2O (L) (in)	H2O (R) (in)	H2O (in)	Qstd (m3/min)	I (chart)	IC corrected	LINEAR REGRESSION
18	5.70	5.70	11.4	1.691	60	59.80	Slope = 33.7639 Intercept = 2.9958 Corr. coeff. = 0.9995
13	4.50	4.50	9.0	1.503	54	53.82	
10	3.50	3.50	7.0	1.326	48	47.84	
7	2.30	2.30	4.6	1.076	40	39.86	
5	1.30	1.30	2.6	0.810	30	29.90	

Calculations :

$$Qstd = 1/m[\text{Sqrt}(H2O(Pa/Pstd)(Tstd/Ta))]-b$$

$$IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$$

Qstd = standard flow rate

IC = corrected chart responses

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)

Pstd = actual pressure during calibration (mm Hg)

For subsequent calculation of sampler flow:

$$1/m((I)[\text{Sqrt}(298/Tav)(Pav/760)]-b)$$


m = sampler slope

b = sampler intercept

I = chart response

Tav = daily average temperature

Pav = daily average pressure

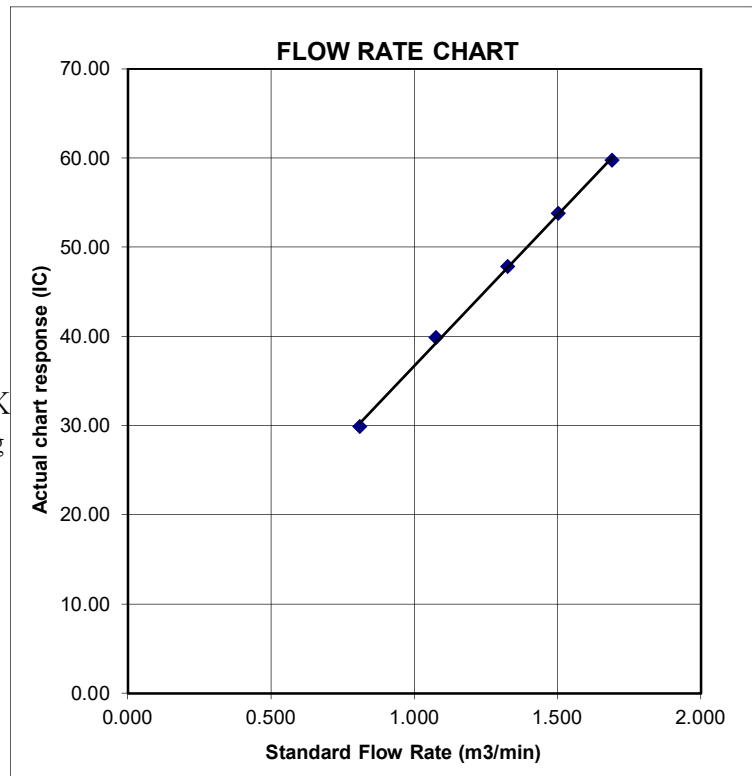

TSP SAMPLER CALIBRATION CALCULATION SPREADSHEET

Location ID : AM2	Date of Calibration: 19-May-22
Name and Model: TISCH HVS Model TE-5170	Next Calibration Date: 19-Jul-22
	Operator: Dixon Chan

CONDITIONS

Sea Level Pressure (hPa) 1011.9	Corrected Pressure (mm Hg) 758.925
Temperature (°C) 25.8	Temperature (K) 299

CALIBRATION ORIFICE

Make-> TISCH	Qstd Slope -> 1.99838
Model-> 5025A	Qstd Intercept -> -0.00903
Serial # -> 1612	

CALIBRATION

Plate No.	H2O (L) (in)	H2O (R) (in)	H2O (in)	Qstd (m3/min)	I (chart)	IC corrected	LINEAR REGRESSION		
							Slope =	Intercept =	Corr. coeff. =
18	6.40	6.40	12.8	1.791	52	51.82	Slope = 31.8110 Intercept = -5.2670 Corr. coeff. = 0.9987		
13	5.10	5.10	10.2	1.599	45	44.85			
10	3.90	3.90	7.8	1.399	40	39.86			
7	2.50	2.50	5.0	1.121	31	30.90			
5	1.50	1.50	3.0	0.869	22	21.93			

Calculations :

$$Qstd = 1/m[\text{Sqrt}(H2O(Pa/Pstd)(Tstd/Ta))-b]$$

$$IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$$

Qstd = standard flow rate

IC = corrected chart responses

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K

Pstd = actual pressure during calibration (mm Hg

For subsequent calculation of sampler flow:

$$1/m((I)[\text{Sqrt}(298/Tav)(Pav/760)]-b)$$


m = sampler slope

b = sampler intercept

I = chart response

Tav = daily average temperature

Pav = daily average pressure

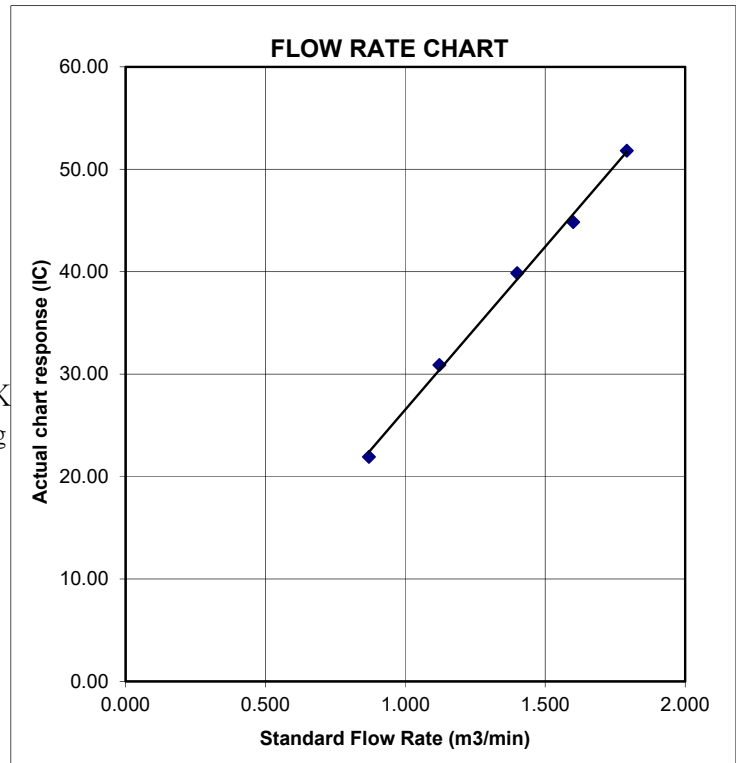

TSP SAMPLER CALIBRATION CALCULATION SPREADSHEET

Location ID : AM3	Date of Calibration: 19-May-22
Name and Model: TISCH HVS Model TE-5170	Next Calibration Date: 19-Jul-22
	Operator: Dixon Chan

CONDITIONS

Sea Level Pressure (hPa) 1011.9	Corrected Pressure (mm Hg) 758.925
Temperature (°C) 25.8	Temperature (K) 299

CALIBRATION ORIFICE

Make-> TISCH	Qstd Slope -> 1.99838
Model-> 5025A	Qstd Intercept -> -0.00903
Serial # -> 1612	

CALIBRATION

Plate No.	H2O (L) (in)	H2O (R) (in)	H2O (in)	Qstd (m3/min)	I (chart)	IC corrected	LINEAR REGRESSION
18	5.40	5.40	10.8	1.646	56	55.81	Slope = 42.8543 Intercept = -14.5250 Corr. coeff. = 0.9965
13	4.00	4.00	8.0	1.417	48	47.84	
10	3.60	3.60	7.2	1.344	42	41.86	
7	2.40	2.40	4.8	1.099	32	31.89	
5	1.40	1.40	2.8	0.840	22	21.93	

Calculations :

$$Qstd = 1/m[\text{Sqrt}(H2O(Pa/Pstd)(Tstd/Ta))-b]$$

$$IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$$

Qstd = standard flow rate

IC = corrected chart responses

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)

Pstd = actual pressure during calibration (mm Hg)

For subsequent calculation of sampler flow:

$$1/m((I)[\text{Sqrt}(298/Tav)(Pav/760)]-b)$$


m = sampler slope

b = sampler intercept

I = chart response

Tav = daily average temperature

Pav = daily average pressure

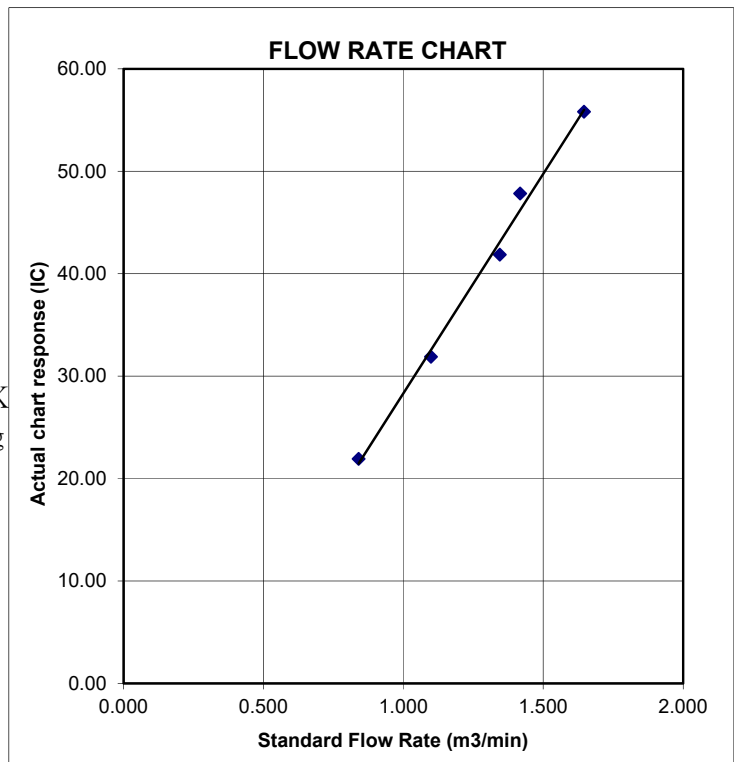

TSP SAMPLER CALIBRATION CALCULATION SPREADSHEET

Location ID : AM4	Date of Calibration: 19-May-22
Name and Model: TISCH HVS Model TE-5170	Next Calibration Date: 19-Jul-22
	Operator: Dixon Chan

CONDITIONS

Sea Level Pressure (hPa) 1011.9	Corrected Pressure (mm Hg) 758.925
Temperature (°C) 25.8	Temperature (K) 299

CALIBRATION ORIFICE

Make-> TISCH	Qstd Slope -> 1.99838
Model-> 5025A	Qstd Intercept -> -0.00903
Serial # -> 1612	

CALIBRATION

Plate No.	H2O (L) (in)	H2O (R) (in)	H2O (in)	Qstd (m3/min)	I (chart)	IC corrected	LINEAR REGRESSION		
							Slope =	Intercept =	Corr. coeff. =
18	6.20	6.20	12.4	1.763	54	53.82	28.3766	3.6780	0.9991
13	4.90	4.90	9.8	1.568	48	47.84			
10	3.80	3.80	7.6	1.381	43	42.85			
7	2.30	2.30	4.6	1.076	35	34.88			
5	1.50	1.50	3.0	0.869	28	27.91			

Calculations :

$$Qstd = 1/m[\text{Sqrt}(H2O(Pa/Pstd)(Tstd/Ta))-b]$$

$$IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$$

Qstd = standard flow rate

IC = corrected chart responses

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)

Pstd = actual pressure during calibration (mm Hg)

For subsequent calculation of sampler flow:

$$1/m((I)[\text{Sqrt}(298/Tav)(Pav/760)]-b)$$

m = sampler slope

b = sampler intercept

I = chart response

Tav = daily average temperature

Pav = daily average pressure

