

Annex D1

# Calibration Certificates for Dust Monitoring Equipment

## TSP SAMPLER CALIBRATION CALCULATION SPREADSHEET

Location ID: AM1	Date of Calibration:	26-Jun-23
Name and Model : TISCH HVS Model TE-5170	Next Calibration Date:	25-Aug-23
	Operator:	P.F.Yeung

### CONDITIONS

Sea Level Pressure (hpa)	1009	Corrected Pressure (mm Hg)	756.8
Temperature (°C)	30.0	Temperature (K)	303

### CALIBRATION ORIFICE

Make:	TISCH	Qstd Slope	2.06918
Model:	TE-5025A	Qstd Intercept	-0.04220
Serial#:	2454		

### CALIBRATION

Plate No.	H2O(L) (in)	H2O(R) (in)	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)	LINEAR REGRESSION
18	5.1	5.1	10.2	1.548	55	54.44	Slope= 32.147 Intercept= 4.931 Corr. Coeff.= 0.9987
13	4.1	4.1	8.2	1.390	50	49.49	
10	2.8	2.7	5.5	1.142	43	42.56	
7	2.0	1.9	3.9	0.965	36	35.64	
5	1.2	1.1	2.3	0.746	29	28.71	

#### Calculations:

$$Qstd = 1/m[\text{Sqrt}(H2O(Pa/Pstd)(Tstd/Ta))-b]$$

$$IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$$

Qstd = standard flow rate

IC = corrected chart response

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)

Pa = actual pressure during calibration (mm Hg)

#### For subsequent calculation of sampler flow:

$$1/m(I[\text{Sqrt}(298/Tav)(Pav/760)]-b)$$


m = sampler slope

b = sampler intercept

I = chart response

Tav = daily average temperature

Pav = daily average pressure

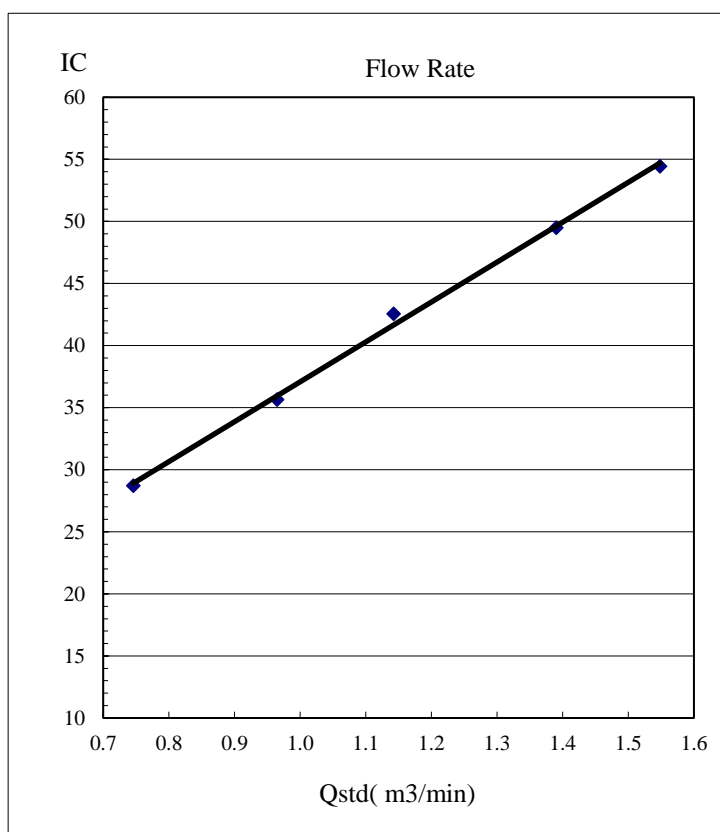

## TSP SAMPLER CALIBRATION CALCULATION SPREADSHEET

Location ID: AM2	Date of Calibration:	26-Jun-23
Name and Model : TISCH HVS Model TE-5170	Next Calibration Date:	25-Aug-23
	Operator:	P.F.Yeung

### CONDITIONS

Sea Level Pressure (hpa)	1009	Corrected Pressure (mm Hg)	756.8
Temperature (°C)	30.0	Temperature (K)	303

### CALIBRATION ORIFICE

Make:	TISCH	Qstd Slope	2.06918
Model:	TE-5025A	Qstd Intercept	-0.04220
Serial#:	2454		

### CALIBRATION

Plate No.	H2O(L) (in)	H2O(R) (in)	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)	LINEAR REGRESSION
18	6.1	6.0	12.1	1.684	53	52.46	Slope= 26.059 Intercept= 8.709 Corr. Coeff.= 0.9952
13	4.5	4.4	8.9	1.448	48	47.51	
10	3.5	3.5	7.0	1.286	42	41.58	
7	2.2	2.3	4.5	1.035	35	34.65	
5	1.2	1.3	2.5	0.777	30	29.70	

#### Calculations:

$$Qstd = 1/m[\text{Sqrt}(H2O(Pa/Pstd)(Tstd/Ta))-b]$$

$$IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$$

Qstd = standard flow rate

IC = corrected chart response

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)

Pa = actual pressure during calibration (mm Hg)

#### For subsequent calculation of sampler flow:

$$1/m(I[\text{Sqrt}(298/Tav)(Pav/760)]-b)$$


m = sampler slope

b = sampler intercept

I = chart response

Tav = daily average temperature

Pav = daily average pressure

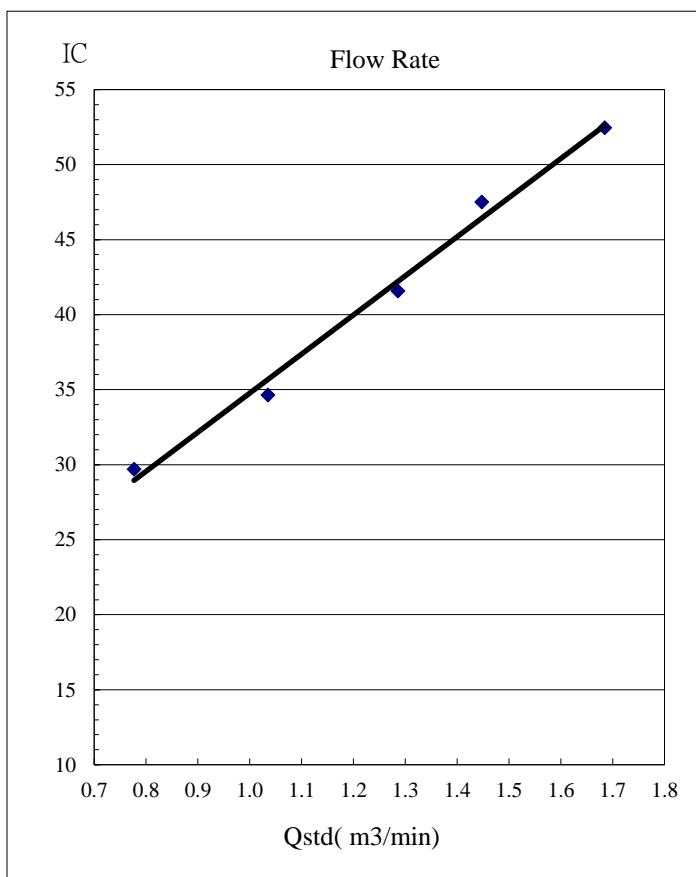

## TSP SAMPLER CALIBRATION CALCULATION SPREADSHEET

Location ID: AM3	Date of Calibration:	26-Jun-23
Name and Model : TISCH HVS Model TE-5170	Next Calibration Date:	25-Aug-23
	Operator:	P.F.Yeung

### CONDITIONS

Sea Level Pressure (hpa)	1009	Corrected Pressure (mm Hg)	756.8
Temperature (°C)	30.0	Temperature (K)	303

### CALIBRATION ORIFICE

Make:	TISCH	Qstd Slope	2.06918
Model:	TE-5025A	Qstd Intercept	-0.04220
Serial#:	2454		

### CALIBRATION

Plate No.	H2O(L) (in)	H2O(R) (in)	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)	LINEAR REGRESSION
18	5.3	5.3	10.6	1.578	60	59.39	Slope= 29.708 Intercept= 11.211 Corr. Coeff.= 0.9953
13	4.6	4.5	9.1	1.464	54	53.45	
10	3.4	3.4	6.8	1.268	49	48.50	
7	2.2	2.2	4.4	1.024	42	41.58	
5	1.3	1.2	2.5	0.777	35	34.65	

#### Calculations:

$$Qstd = 1/m[\text{Sqrt}(H2O(Pa/Pstd)(Tstd/Ta))-b]$$

$$IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$$

Qstd = standard flow rate

IC = corrected chart response

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)

Pa = actual pressure during calibration (mm Hg)

#### For subsequent calculation of sampler flow:

$$1/m(I[\text{Sqrt}(298/Tav)(Pav/760)]-b)$$


m = sampler slope

b = sampler intercept

I = chart response

Tav = daily average temperature

Pav = daily average pressure

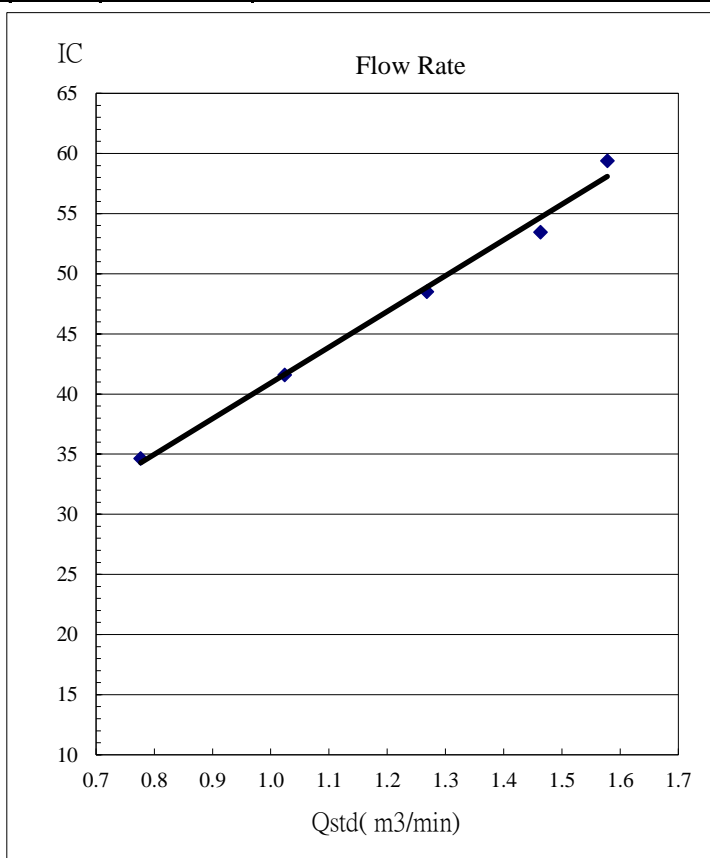

## TSP SAMPLER CALIBRATION CALCULATION SPREADSHEET

Location ID: AM4	Date of Calibration:	26-Jun-23
Name and Model : TISCH HVS Model TE-5170	Next Calibration Date:	25-Aug-23
	Operator:	P.F.Yeung

### CONDITIONS

Sea Level Pressure (hpa)	1009	Corrected Pressure (mm Hg)	756.8
Temperature (°C)	30.0	Temperature (K)	303

### CALIBRATION ORIFICE

Make:	TISCH	Qstd Slope	2.06918
Model:	TE-5025A	Qstd Intercept	-0.04220
Serial#:	2454		

### CALIBRATION

Plate No.	H2O(L) (in)	H2O(R) (in)	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)	LINEAR REGRESSION
18	6.1	6.1	12.2	1.691	57	56.42	Slope= 31.719 Intercept= 3.367 Corr. Coeff.= 0.998
13	4.6	4.5	9.1	1.464	51	50.48	
10	3.6	3.6	7.2	1.304	45	44.54	
7	2.2	2.2	4.4	1.024	37	36.63	
5	1.4	1.4	2.8	0.821	29	28.71	

#### Calculations:

$$Qstd = 1/m[\text{Sqrt}(H2O(Pa/Pstd)(Tstd/Ta))-b]$$

$$IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$$

Qstd = standard flow rate

IC = corrected chart response

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)

Pa = actual pressure during calibration (mm Hg)

#### For subsequent calculation of sampler flow:

$$1/m(I[\text{Sqrt}(298/Tav)(Pav/760)]-b)$$

m = sampler slope

b = sampler intercept

I = chart response

Tav = daily average temperature

Pav = daily average pressure

