



ANNEX D1

CALIBRATION CERTIFICATES FOR DUST
MONITORING EQUIPMENT

TSP SAMPLER CALIBRATION CACULATION SPREADSHEET

Location ID: AM1 Name and Model : TISCH HVS Model TE-5170		Date of Calibration: 24-Oct-23 Next Calibration Date: 23-Dec-23 Operator: P.F.Yeung					
CONDITIONS							
Sea Level Pressure (hpa) Temperature (°C)	1016 20.6	Corrected Pressure (mm Hg) Temperature (K)	762.1 299				
CALIBRATION ORIFICE							
Make: Model: Serial#:	TISCH TE-5025A 2454	Qstd Slope Qstd Intercept	2.06918 -0.04220				
CALIBRATION							
Plate No.	H2O(L) (in)	H2O(R) (in)	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)	LINEAR REGRESSION
18	5.6	5.7	11.3	1.645	56	56.00	Slope= 32.550
13	4.0	3.9	7.9	1.379	51	51.00	Intercept= 4.006
10	3.1	3.0	6.1	1.214	44	44.00	Corr. Coeff.= 0.9915
7	2.1	2.0	4.1	0.999	36	36.00	
5	1.4	1.3	2.7	0.814	30	30.00	
Calulations:							
$Q_{std} = 1/m[\sqrt{H_2O(P_a/P_{std})(T_{std}/T_a)} - b]$							
$IC = I[\sqrt{P_a/P_{std}}(T_{std}/T_a)]$							
<p>Q_{std} = standard flow rate IC = corrected chart response I = actual chart response m = calibrator Q_{std} slope b = calibrator Q_{std} intercept T_a = actual temperature during calibration (deg K) P_a = actual pressure during calibration (mm Hg)</p>							
<p>For subsequent calculation of sampler flow:</p> $1/m((I)[\sqrt{298/T_{avg}}(\bar{P}_a/760)] - b)$ <p>m = sampler slope b = sampler intercept I = chart response T_{avg} = daily average temperature \bar{P}_a = daily average pressure</p>							

TSP SAMPLER CALIBRATION CACULATION SPREADSHEET

Location ID: AM2 Name and Model : TISCH HVS Model TE-5170	Date of Calibration: 24-Oct-23 Next Calibration Date: 23-Dec-23 Operator: P.F.Yeung							
CONDITIONS								
Sea Level Pressure (hpa) Temperature (°C)	<table border="1" style="display: inline-table; vertical-align: middle;"> <tr><td>1016</td></tr> <tr><td>26.0</td></tr> </table>	1016	26.0	Corrected Pressure (mm Hg) Temperature (K)	<table border="1" style="display: inline-table; vertical-align: middle;"> <tr><td>762.1</td></tr> <tr><td>299</td></tr> </table>	762.1	299	
1016								
26.0								
762.1								
299								
CALIBRATION ORIFICE								
Make: Model: Serial#:	<table border="1" style="display: inline-table; vertical-align: middle;"> <tr><td>TISCH</td></tr> <tr><td>TE-5025A</td></tr> <tr><td>2454</td></tr> </table>	TISCH	TE-5025A	2454	Qstd Slope Qstd Intercept	<table border="1" style="display: inline-table; vertical-align: middle;"> <tr><td>2.06918</td></tr> <tr><td>-0.04220</td></tr> </table>	2.06918	-0.04220
TISCH								
TE-5025A								
2454								
2.06918								
-0.04220								
CALIBRATION								
Plate No.	H2O(L) (in)	H2O(R) (in)	H2O (in)	Qstd (m ³ /min)	I (chart)	IC (corrected)	LINEAR REGRESSION	
18	6.0	5.9	11.9	1.687	53	53.00	Slope= 25.811	
13	4.4	4.3	8.7	1.446	48	48.00	Intercept= 10.384	
10	3.0	3.0	6.0	1.204	43	43.00	Corr. Coeff.= 0.9935	
7	2.0	2.0	4.0	0.987	36	36.00		
5	1.3	1.3	2.6	0.800	30	30.00		

Calulations:

$Q_{std} = 1/m[\sqrt{H_2O(P_a/P_{std})(T_{std}/T_a)} - b]$

$IC = I[\sqrt{P_a/P_{std}}(T_{std}/T_a)]$

Q_{std} = standard flow rate
 IC = corrected chart response
 I = actual chart response
 m = calibrator Q_{std} slope
 b = calibrator Q_{std} intercept
 T_a = actual temperature during calibration (deg K)
 P_a = actual pressure during calibration (mm Hg)

For subsequent calculation of sampler flow:

$1/m(I)[\sqrt{(298/T_{avg})(P_{avg}/760)}] - b$

m = sampler slope
 b = sampler intercept
 I = chart response
 T_{avg} = daily average temperature
 P_{avg} = daily average pressure

Flow Rate

Qstd (m ³ /min)	IC
0.80	30.00
1.00	35.00
1.20	43.00
1.40	48.00
1.70	54.00

TSP SAMPLER CALIBRATION CACULATION SPREADSHEET

Location ID: AM3 Name and Model : TISCH HVS Model TE-5170	Date of Calibration: 24-Oct-23 Next Calibration Date: 23-Dec-23 Operator: P.F.Yeung							
CONDITIONS								
Sea Level Pressure (hpa) Temperature (°C)	<table border="1" style="display: inline-table; vertical-align: middle;"> <tr><td>1016</td></tr> <tr><td>26.0</td></tr> </table>	1016	26.0	Corrected Pressure (mm Hg) Temperature (K)	<table border="1" style="display: inline-table; vertical-align: middle;"> <tr><td>762.1</td></tr> <tr><td>299</td></tr> </table>	762.1	299	
1016								
26.0								
762.1								
299								
CALIBRATION ORIFICE								
Make: Model: Serial#:	<table border="1" style="display: inline-table; vertical-align: middle;"> <tr><td>TISCH</td></tr> <tr><td>TE-5025A</td></tr> <tr><td>2454</td></tr> </table>	TISCH	TE-5025A	2454	Qstd Slope Qstd Intercept	<table border="1" style="display: inline-table; vertical-align: middle;"> <tr><td>2.06918</td></tr> <tr><td>-0.04220</td></tr> </table>	2.06918	-0.04220
TISCH								
TE-5025A								
2454								
2.06918								
-0.04220								
CALIBRATION								
Plate No.	H2O(L) (in)	H2O(R) (in)	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)	LINEAR REGRESSION	
18	5.9	5.8	11.7	1.673	57	57.00	Slope= 27.980	
13	4.6	4.5	9.1	1.478	52	52.00	Intercept= 10.675	
10	3.2	3.2	6.4	1.243	46	46.00	Corr. Coeff.= 0.9964	
7	2.1	2.1	4.2	1.011	40	40.00		
5	1.3	1.3	2.6	0.800	32	32.00		

Calulations:

Qstd = $1/m[\text{Sqrt}(H2O(Pa/Pstd)(Tstd/Ta))-b]$
 IC = $I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$

Qstd = standard flow rate
 IC = corrected chart response
 I = actual chart response
 m = calibrator Qstd slope
 b = calibrator Qstd intercept
 Ta = actual temperature during calibration (deg K)
 Pa = actual pressure during calibration (mm Hg)

For subsequent calculation of sampler flow:
 $1/m(I)[\text{Sqrt}(298/Tav)(Pav/760)]-b$

m = sampler slope
 b = sampler intercept
 I = chart response
 Tav = daily average temperature
 Pav = daily average pressure

Qstd (m3/min)	IC
0.80	33.0
1.00	40.0
1.20	46.0
1.50	52.0
1.70	57.0

TSP SAMPLER CALIBRATION CACULATION SPREADSHEET

Location ID: AM4 Name and Model : TISCH HVS Model TE-5170		Date of Calibration: 24-Oct-23 Next Calibration Date: 23-Dec-23 Operator: P.F.Yeung					
CONDITIONS							
Sea Level Pressure (hpa) Temperature (°C)	1016 26.0	Corrected Pressure (mm Hg) Temperature (K)	762.1 299				
CALIBRATION ORIFICE							
Make: Model: Serial#:	TISCH TE-5025A 2454	Qstd Slope Qstd Intercept	2.06918 -0.04220				
CALIBRATION							
Plate No.	H2O(L) (in)	H2O(R) (in)	H2O (in)	Qstd (m³/min)	I (chart)	IC (corrected)	LINEAR REGRESSION
18	6.1	6.2	12.3	1.715	58	58.00	Slope= 31.691
13	4.8	4.8	9.6	1.518	52	52.00	Intercept= 3.979
10	3.5	3.5	7.0	1.299	46	46.00	Corr. Coeff.= 0.9991
7	2.4	2.4	4.8	1.079	38	38.00	
5	1.4	1.4	2.8	0.829	30	30.00	
Calulations:							
$Q_{std} = 1/m[\sqrt{H_2O(Pa/Pstd)(Tstd/Ta)} - b]$							
$IC = I[\sqrt{Pa/Pstd}(Tstd/Ta)]$							
<p>Q_{std} = standard flow rate IC = corrected chart response I = actual chart response m = calibrator Q_{std} slope b = calibrator Q_{std} intercept Ta = actual temperature during calibration (deg K) Pa = actual pressure during calibration (mm Hg)</p>							
<p>For subsequent calculation of sampler flow:</p> $1/m(I)[\sqrt{(298/Tav)(Pav/760)}] - b$ <p>m = sampler slope b = sampler intercept I = chart response Tav = daily average temperature Pav = daily average pressure</p>							

TSP SAMPLER CALIBRATION CACULATION SPREADSHEET

Location ID: AM1 Name and Model : TISCH HVS Model TE-5170	Date of Calibration: 22-Dec-23 Next Calibration Date: 21-Feb-24 Operator: P.F.Yeung							
CONDITIONS								
Sea Level Pressure (hpa) Temperature (°C)	<table border="1" style="display: inline-table; vertical-align: middle;"> <tr><td>1027</td></tr> <tr><td>10.0</td></tr> </table>	1027	10.0	Corrected Pressure (mm Hg) Temperature (K)	<table border="1" style="display: inline-table; vertical-align: middle;"> <tr><td>770.3</td></tr> <tr><td>283</td></tr> </table>	770.3	283	
1027								
10.0								
770.3								
283								
CALIBRATION ORIFICE								
Make: Model: Serial#:	<table border="1" style="display: inline-table; vertical-align: middle;"> <tr><td>TISCH</td></tr> <tr><td>TE-5025A</td></tr> <tr><td>2454</td></tr> </table>	TISCH	TE-5025A	2454	Qstd Slope Qstd Intercept	<table border="1" style="display: inline-table; vertical-align: middle;"> <tr><td>2.07544</td></tr> <tr><td>-0.03205</td></tr> </table>	2.07544	-0.03205
TISCH								
TE-5025A								
2454								
2.07544								
-0.03205								
CALIBRATION								
Plate No.	H2O(L) (in)	H2O(R) (in)	H2O (in)	Qstd (m ³ /min)	I (chart)	IC (corrected)	LINEAR REGRESSION	
18	5.3	5.3	10.6	1.636	56	57.87	Slope= 28.984	
13	4.3	4.4	8.7	1.484	50	51.67	Intercept= 9.8992	
10	3.0	2.9	5.9	1.225	45	46.50	Corr. Coeff.= 0.9959	
7	2.0	2.1	4.1	1.024	38	39.27		
5	1.2	1.3	2.5	0.803	32	33.07		

Calulations:

$Q_{std} = 1/m[\sqrt{H_2O(P_a/P_{std})(T_{std}/T_a)} - b]$


$IC = I[\sqrt{P_a/P_{std}}(T_{std}/T_a)]$

Q_{std} = standard flow rate
 IC = corrected chart response
 I = actual chart response
 m = calibrator Q_{std} slope
 b = calibrator Q_{std} intercept
 T_a = actual temperature during calibration (deg K)
 P_a = actual pressure during calibration (mm Hg)

For subsequent calculation of sampler flow:

$1/m((I)[\sqrt{298/T_{avg}}(P_{avg}/760)] - b)$

m = sampler slope
 b = sampler intercept
 I = chart response
 T_{avg} = daily average temperature
 P_{avg} = daily average pressure

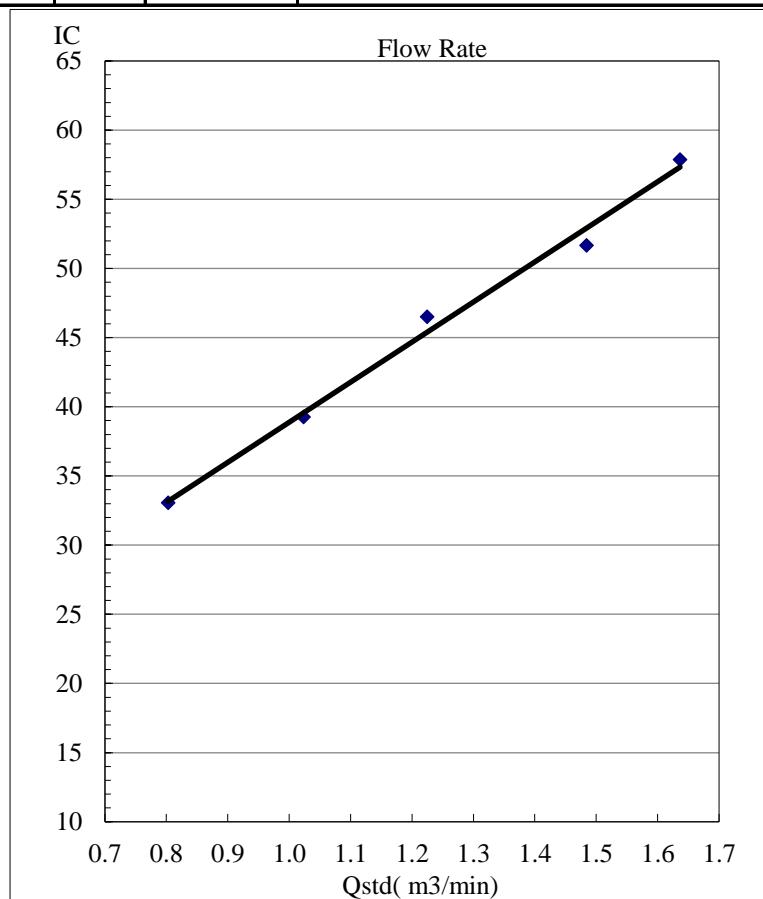

TSP SAMPLER CALIBRATION CACULATION SPREADSHEET

Location ID: AM2 Name and Model : TISCH HVS Model TE-5170	Date of Calibration: 22-Dec-23 Next Calibration Date: 21-Feb-24 Operator: P.F.Yeung							
CONDITIONS								
Sea Level Pressure (hpa) Temperature (°C)	<table border="1" style="display: inline-table; vertical-align: middle;"> <tr><td>1027</td></tr> <tr><td>10.0</td></tr> </table>	1027	10.0	Corrected Pressure (mm Hg) Temperature (K)	<table border="1" style="display: inline-table; vertical-align: middle;"> <tr><td>770.3</td></tr> <tr><td>283</td></tr> </table>	770.3	283	
1027								
10.0								
770.3								
283								
CALIBRATION ORIFICE								
Make: Model: Serial#:	<table border="1" style="display: inline-table; vertical-align: middle;"> <tr><td>TISCH</td></tr> <tr><td>TE-5025A</td></tr> <tr><td>2454</td></tr> </table>	TISCH	TE-5025A	2454	Qstd Slope Qstd Intercept	<table border="1" style="display: inline-table; vertical-align: middle;"> <tr><td>2.07544</td></tr> <tr><td>-0.03205</td></tr> </table>	2.07544	-0.03205
TISCH								
TE-5025A								
2454								
2.07544								
-0.03205								
CALIBRATION								
Plate No.	H2O(L) (in)	H2O(R) (in)	H2O (in)	Qstd (m ³ /min)	I (chart)	IC (corrected)	LINEAR REGRESSION	
18	6.1	6.1	12.2	1.755	52	53.73	Slope= 26.430	
13	4.9	4.9	9.8	1.574	48	49.60	Intercept= 7.718	
10	3.6	3.6	7.2	1.351	43	44.43	Corr. Coeff.= 0.9952	
7	2.5	2.5	5.0	1.129	35	36.17		
5	1.4	1.5	2.9	0.863	30	31.00		

Calculations:

$Q_{std} = 1/m[\sqrt{H_2O(P_a/P_{std})(T_{std}/T_a)} - b]$

$IC = I[\sqrt{P_a/P_{std}}(T_{std}/T_a)]$

$Q_{std} = \text{standard flow rate}$
 $IC = \text{corrected chart response}$
 $I = \text{actual chart response}$
 $m = \text{calibrator } Q_{std} \text{ slope}$
 $b = \text{calibrator } Q_{std} \text{ intercept}$
 $T_a = \text{actual temperature during calibration (deg K)}$
 $P_a = \text{actual pressure during calibration (mm Hg)}$

For subsequent calculation of sampler flow:

$1/m((I)[\sqrt{298/T_{avg}}(P_{avg}/760)] - b)$

$m = \text{sampler slope}$
 $b = \text{sampler intercept}$
 $I = \text{chart response}$
 $T_{avg} = \text{daily average temperature}$
 $P_{avg} = \text{daily average pressure}$

TSP SAMPLER CALIBRATION CACULATION SPREADSHEET

Location ID: AM3 Name and Model : TISCH HVS Model TE-5170	Date of Calibration: 22-Dec-23 Next Calibration Date: 21-Feb-24 Operator: P.F.Yeung							
CONDITIONS								
Sea Level Pressure (hpa) Temperature (°C)	<table border="1" style="display: inline-table; vertical-align: middle;"> <tr><td>1027</td></tr> <tr><td>10.0</td></tr> </table>	1027	10.0	Corrected Pressure (mm Hg) Temperature (K)	<table border="1" style="display: inline-table; vertical-align: middle;"> <tr><td>770.3</td></tr> <tr><td>283</td></tr> </table>	770.3	283	
1027								
10.0								
770.3								
283								
CALIBRATION ORIFICE								
Make: Model: Serial#:	<table border="1" style="display: inline-table; vertical-align: middle;"> <tr><td>TISCH</td></tr> <tr><td>TE-5025A</td></tr> <tr><td>2454</td></tr> </table>	TISCH	TE-5025A	2454	Qstd Slope Qstd Intercept	<table border="1" style="display: inline-table; vertical-align: middle;"> <tr><td>2.07544</td></tr> <tr><td>-0.03205</td></tr> </table>	2.07544	-0.03205
TISCH								
TE-5025A								
2454								
2.07544								
-0.03205								
CALIBRATION								
Plate No.	H2O(L) (in)	H2O(R) (in)	H2O (in)	Qstd (m ³ /min)	I (chart)	IC (corrected)	LINEAR REGRESSION	
18	5.9	5.9	11.8	1.726	56	57.87	Slope= 23.822	
13	4.6	4.7	9.3	1.534	51	52.70	Intercept= 16.621	
10	3.3	3.2	6.5	1.285	46	47.53	Corr. Coeff.= 0.9991	
7	2.1	2.0	4.1	1.024	40	41.33		
5	1.3	1.4	2.7	0.834	35	36.17		

Calulations:

$Q_{std} = 1/m[\sqrt{H_2O(P_a/P_{std})(T_{std}/T_a)} - b]$

$IC = I[\sqrt{P_a/P_{std}}(T_{std}/T_a)]$

Q_{std} = standard flow rate
 IC = corrected chart response
 I = actual chart response
 m = calibrator Q_{std} slope
 b = calibrator Q_{std} intercept
 T_a = actual temperature during calibration (deg K)
 P_a = actual pressure during calibration (mm Hg)

For subsequent calculation of sampler flow:

$1/m((I)[\sqrt{298/T_{avg}}(P_{avg}/760)] - b)$

m = sampler slope
 b = sampler intercept
 I = chart response
 T_{avg} = daily average temperature
 P_{avg} = daily average pressure

Flow Rate

Qstd (m ³ /min)	IC
0.834	36.17
1.024	41.33
1.285	47.53
1.534	52.70
1.726	57.87

TSP SAMPLER CALIBRATION CACULATION SPREADSHEET

Location ID: AM4 Name and Model : TISCH HVS Model TE-5170	Date of Calibration: 22-Dec-23 Next Calibration Date: 21-Feb-24 Operator: P.F.Yeung							
CONDITIONS								
Sea Level Pressure (hpa) Temperature (°C)	<table border="1" style="display: inline-table; vertical-align: middle;"> <tr><td>1027</td></tr> <tr><td>10.0</td></tr> </table>	1027	10.0	Corrected Pressure (mm Hg) Temperature (K)	<table border="1" style="display: inline-table; vertical-align: middle;"> <tr><td>770.3</td></tr> <tr><td>283</td></tr> </table>	770.3	283	
1027								
10.0								
770.3								
283								
CALIBRATION ORIFICE								
Make: Model: Serial#:	<table border="1" style="display: inline-table; vertical-align: middle;"> <tr><td>TISCH</td></tr> <tr><td>TE-5025A</td></tr> <tr><td>2454</td></tr> </table>	TISCH	TE-5025A	2454	Qstd Slope Qstd Intercept	<table border="1" style="display: inline-table; vertical-align: middle;"> <tr><td>2.07544</td></tr> <tr><td>-0.03205</td></tr> </table>	2.07544	-0.03205
TISCH								
TE-5025A								
2454								
2.07544								
-0.03205								
CALIBRATION								
Plate No.	H2O(L) (in)	H2O(R) (in)	H2O (in)	Qstd (m ³ /min)	I (chart)	IC (corrected)	LINEAR REGRESSION	
18	6.4	6.5	12.9	1.804	58	59.93	Slope= 30.977	
13	4.6	4.5	9.1	1.517	52	53.73	Intercept= 4.808	
10	3.7	3.7	7.4	1.370	45	46.50	Corr. Coeff.= 0.9950	
7	2.2	2.3	4.5	1.072	36	37.20		
5	1.3	1.4	2.7	0.834	30	31.00		

Calulations:

$Q_{std} = 1/m[\sqrt{H_2O(P_a/P_{std})(T_{std}/T_a)} - b]$

$IC = I[\sqrt{P_a/P_{std}}(T_{std}/T_a)]$

Q_{std} = standard flow rate
 IC = corrected chart response
 I = actual chart response
 m = calibrator Q_{std} slope
 b = calibrator Q_{std} intercept
 Ta = actual temperature during calibration (deg K)
 Pa = actual pressure during calibration (mm Hg)

For subsequent calculation of sampler flow:
 $1/m(I)[\sqrt{(298/T_{avg})(P_{avg}/760)}] - b$

m = sampler slope
 b = sampler intercept
 I = chart response
 T_{avg} = daily average temperature
 P_{avg} = daily average pressure

Qstd (m ³ /min)	IC
0.80	31.00
1.10	37.20
1.50	53.73
1.80	60.00