



ANNEX D1

CALIBRATION CERTIFICATES FOR DUST  
MONITORING EQUIPMENT

# TSP SAMPLER CALIBRATION CACULATION SPREADSHEET

Location ID: AM1 Name and Model : TISCH HVS Model TE-5170		Date of Calibration: 22-Apr-24 Next Calibration Date: 22-Jun-24 Operator: P.F.Yeung					
<b>CONDITIONS</b>							
Temperature (°C)	1014 25.0	Corrected Pressure (mm Hg) Temperature (K)	760.1 298				
<b>CALIBRATION ORIFICE</b>							
Make:	TISCH	Qstd Slope	2.07544				
Model:	TE-5025A	Qstd Intercept	-0.03205				
Serial#:	2454						
<b>CALIBRATION</b>							
Plate No.	H2O(L) (in)	H2O(R) (in)	H2O (in)	Qstd (m³/min)	I (chart)	IC (corrected)	LINEAR REGRESSION
18	5.4	5.4	10.8	1.600	52	52.03	Slope= 33.386
13	4.4	4.4	8.8	1.446	47	47.03	Intercept= -0.9831
10	2.9	3.0	5.9	1.187	40	40.02	Corr. Coeff.= 0.9974
7	2.2	2.2	4.4	1.027	33	33.02	
5	1.3	1.3	2.6	0.793	25	25.02	
<b>Calulations:</b>							
$Q_{std} = 1/m[\sqrt{H_2O(P_a/P_{std})(T_{std}/T_a)} - b]$							
$IC = I[\sqrt{P_a/P_{std}}(T_{std}/T_a)]$							
$Q_{std}$ = standard flow rate							
$IC$ = corrected chart response							
$I$ = actual chart response							
$m$ = calibrator $Q_{std}$ slope							
$b$ = calibrator $Q_{std}$ intercept							
$T_a$ = actual temperature during calibration (deg K)							
$P_a$ = actual pressure during calibration (mm Hg)							
<b>For subsequent calculation of sampler flow:</b>							
$1/m(I)[\sqrt{(298/T_{avg})(P_{avg}/760)}] - b$							
$m$ = sampler slope							
$b$ = sampler intercept							
$I$ = chart response							
$T_{avg}$ = daily average temperature							
$P_{avg}$ = daily average pressure							

**Flow Rate**

Qstd (m³/min)	IC
0.80	25.0
1.00	33.0
1.20	40.0
1.60	52.0

# TSP SAMPLER CALIBRATION CACULATION SPREADSHEET

Location ID: AM2 Name and Model : TISCH HVS Model TE-5170	Date of Calibration: 22-Apr-24 Next Calibration Date: 22-Jun-24 Operator: P.F.Yeung							
<b>CONDITIONS</b>								
Sea Level Pressure (hpa) Temperature (°C)	<table border="1" style="display: inline-table; vertical-align: middle;"> <tr><td>1014</td></tr> <tr><td>25.0</td></tr> </table>	1014	25.0	Corrected Pressure (mm Hg) Temperature (K)	<table border="1" style="display: inline-table; vertical-align: middle;"> <tr><td>760.1</td></tr> <tr><td>298</td></tr> </table>	760.1	298	
1014								
25.0								
760.1								
298								
<b>CALIBRATION ORIFICE</b>								
Make: Model: Serial#:	<table border="1" style="display: inline-table; vertical-align: middle;"> <tr><td>TISCH</td></tr> <tr><td>TE-5025A</td></tr> <tr><td>2454</td></tr> </table>	TISCH	TE-5025A	2454	Qstd Slope Qstd Intercept	<table border="1" style="display: inline-table; vertical-align: middle;"> <tr><td>2.07544</td></tr> <tr><td>-0.03205</td></tr> </table>	2.07544	-0.03205
TISCH								
TE-5025A								
2454								
2.07544								
-0.03205								
<b>CALIBRATION</b>								
Plate No.	H2O(L) (in)	H2O(R) (in)	H2O (in)	Qstd (m <sup>3</sup> /min)	I (chart)	IC (corrected)	LINEAR REGRESSION	
18	5.0	5.0	10.0	1.540	52	52.03	Slope= 30.764	
13	4.3	4.3	8.6	1.429	47	47.03	Intercept= 3.559	
10	3.5	3.5	7.0	1.291	42	42.03	Corr. Coeff.= 0.9953	
7	2.1	2.1	4.2	1.004	35	35.02		
5	1.3	1.3	2.6	0.793	28	28.02		

**Calulations:**

$Q_{std} = 1/m[\sqrt{H_2O(Pa/Pstd)(Tstd/Ta)} - b]$

$IC = I[\sqrt{Pa/Pstd}(Tstd/Ta)]$

$Q_{std}$  = standard flow rate  
 $IC$  = corrected chart response  
 $I$  = actual chart response  
 $m$  = calibrator  $Q_{std}$  slope  
 $b$  = calibrator  $Q_{std}$  intercept  
 $Ta$  = actual temperature during calibration (deg K)  
 $Pa$  = actual pressure during calibration (mm Hg)

**For subsequent calculation of sampler flow:**

$1/m(I)[\sqrt{(298/Tav)(Pav/760)}] - b$

$m$  = sampler slope  
 $b$  = sampler intercept  
 $I$  = chart response  
 $Tav$  = daily average temperature  
 $Pav$  = daily average pressure

**Flow Rate**

Qstd (m <sup>3</sup> /min)	IC
0.8	28
1.0	35
1.3	42
1.4	47
1.55	52

# TSP SAMPLER CALIBRATION CACULATION SPREADSHEET

Location ID: AM3 Name and Model : TISCH HVS Model TE-5170	Date of Calibration: 22-Apr-24 Next Calibration Date: 23-Jun-24 Operator: P.F.Yeung							
<b>CONDITIONS</b>								
Sea Level Pressure (hpa) Temperature (°C)	<table border="1" style="display: inline-table; vertical-align: middle;"> <tr><td>1014</td></tr> <tr><td>25.0</td></tr> </table>	1014	25.0	Corrected Pressure (mm Hg) Temperature (K)	<table border="1" style="display: inline-table; vertical-align: middle;"> <tr><td>760.1</td></tr> <tr><td>298</td></tr> </table>	760.1	298	
1014								
25.0								
760.1								
298								
<b>CALIBRATION ORIFICE</b>								
Make: Model: Serial#:	<table border="1" style="display: inline-table; vertical-align: middle;"> <tr><td>TISCH</td></tr> <tr><td>TE-5025A</td></tr> <tr><td>2454</td></tr> </table>	TISCH	TE-5025A	2454	Qstd Slope Qstd Intercept	<table border="1" style="display: inline-table; vertical-align: middle;"> <tr><td>2.07544</td></tr> <tr><td>-0.03205</td></tr> </table>	2.07544	-0.03205
TISCH								
TE-5025A								
2454								
2.07544								
-0.03205								
<b>CALIBRATION</b>								
Plate No.	H2O(L) (in)	H2O(R) (in)	H2O (in)	Qstd (m <sup>3</sup> /min)	I (chart)	IC (corrected)	LINEAR REGRESSION	
18	5.5	5.5	11.0	1.614	57	57.04	Slope= 26.552	
13	4.2	4.2	8.4	1.413	52	52.03	Intercept= 14.177	
10	3.4	3.4	6.8	1.273	47	47.03	Corr. Coeff.= 0.9952	
7	2.1	2.1	4.2	1.004	42	42.03		
5	1.3	1.4	2.7	0.808	35	35.02		

**Calulations:**

$Q_{std} = 1/m[\sqrt{H_2O(P_a/P_{std})(T_{std}/T_a)} - b]$


$IC = I[\sqrt{P_a/P_{std}}(T_{std}/T_a)]$

$Q_{std}$  = standard flow rate  
 $IC$  = corrected chart response  
 $I$  = actual chart response  
 $m$  = calibrator  $Q_{std}$  slope  
 $b$  = calibrator  $Q_{std}$  intercept  
 $T_a$  = actual temperature during calibration (deg K)  
 $P_a$  = actual pressure during calibration (mm Hg)

**For subsequent calculation of sampler flow:**

$1/m(I)[\sqrt{(298/T_{avg})(P_{avg}/760)}] - b$

$m$  = sampler slope  
 $b$  = sampler intercept  
 $I$  = chart response  
 $T_{avg}$  = daily average temperature  
 $P_{avg}$  = daily average pressure

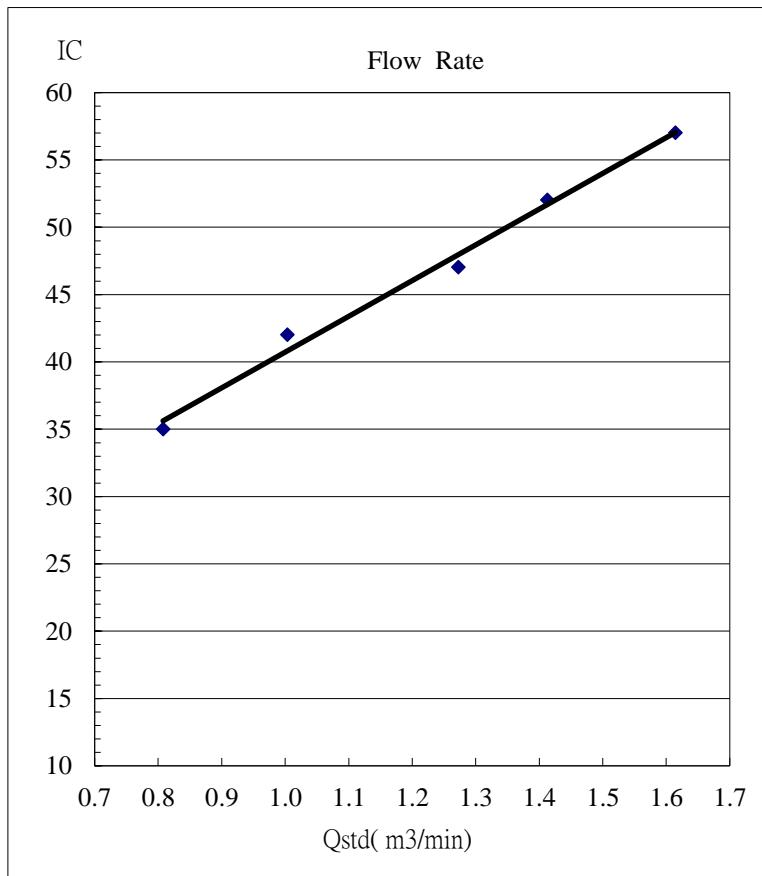

# TSP SAMPLER CALIBRATION CACULATION SPREADSHEET

Location ID: AM4 Name and Model : TISCH HVS Model TE-5170	Date of Calibration: 22-Apr-24 Next Calibration Date: 23-Jun-24 Operator: P.F.Yeung							
<b>CONDITIONS</b>								
Sea Level Pressure (hpa) Temperature (°C)	<table border="1" style="display: inline-table; vertical-align: middle;"> <tr><td>1014</td></tr> <tr><td>25.0</td></tr> </table>	1014	25.0	Corrected Pressure (mm Hg) Temperature (K)	<table border="1" style="display: inline-table; vertical-align: middle;"> <tr><td>760.1</td></tr> <tr><td>298</td></tr> </table>	760.1	298	
1014								
25.0								
760.1								
298								
<b>CALIBRATION ORIFICE</b>								
Make: Model: Serial#:	<table border="1" style="display: inline-table; vertical-align: middle;"> <tr><td>TISCH</td></tr> <tr><td>TE-5025A</td></tr> <tr><td>2454</td></tr> </table>	TISCH	TE-5025A	2454	Qstd Slope Qstd Intercept	<table border="1" style="display: inline-table; vertical-align: middle;"> <tr><td>2.07544</td></tr> <tr><td>-0.03205</td></tr> </table>	2.07544	-0.03205
TISCH								
TE-5025A								
2454								
2.07544								
-0.03205								
<b>CALIBRATION</b>								
Plate No.	H2O(L) (in)	H2O(R) (in)	H2O (in)	Qstd (m <sup>3</sup> /min)	I (chart)	IC (corrected)	LINEAR REGRESSION	
18	6.5	6.4	12.9	1.747	59	59.04	Slope= 32.028	
13	5.1	5.2	10.3	1.563	52	52.03	Intercept= 2.6869	
10	3.8	3.9	7.7	1.353	46	46.03	Corr. Coeff.= 0.9989	
7	2.5	2.4	4.9	1.083	38	38.02		
5	1.6	1.5	3.1	0.864	30	30.02		

**Calulations:**

Qstd =  $1/m[\sqrt{H2O(Pa/Pstd)(Tstd/Ta)} - b]$   
 IC =  $I[\sqrt{Pa/Pstd}(Tstd/Ta)]$

Qstd = standard flow rate  
 IC = corrected chart response  
 I = actual chart response  
 m = calibrator Qstd slope  
 b = calibrator Qstd intercept  
 Ta = actual temperature during calibration (deg K)  
 Pa = actual pressure during calibration (mm Hg)

For subsequent calculation of sampler flow:  
 $1/m(I)[\sqrt{(298/Tav)(Pav/760)}] - b$

m = sampler slope  
 b = sampler intercept  
 I = chart response  
 Tav = daily average temperature  
 Pav = daily average pressure

**IC**                           **Flow Rate**

Qstd (m <sup>3</sup> /min)	IC
0.864	30.02
1.083	38.02
1.353	46.03
1.563	52.03
1.747	59.04