



ANNEX D1

CALIBRATION CERTIFICATES FOR DUST
MONITORING EQUIPMENT

TSP SAMPLER CALIBRATION CALCULATION SPREADSHEET

Location ID: AM1	Date of Calibration:	16-Dec-24
Name and Model : TISCH HVS Model TE-5170	Next Calibration Date:	16-Feb-25
	Operator:	P.F.Yeung

CONDITIONS

	1022.7	Corrected Pressure (mm Hg)	767.1
Temperature (°C)	17.0	Temperature (K)	290

CALIBRATION ORIFICE

Make:	TISCH	Qstd Slope	2.08315
Model:	TE-5025A	Qstd Intercept	-0.04938
Serial#:	2454		

CALIBRATION

Plate No.	H2O(L) (in)	H2O(R) (in)	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)	LINEAR REGRESSION
18	5.6	5.6	11.2	1.660	54	55.01	Slope= 35.201 Intercept= -2.7305 Corr. Coeff.= 0.9953
13	4.4	4.4	8.8	1.474	48	48.90	
10	3.2	3.2	6.4	1.261	42	42.78	
7	2.1	2.1	4.2	1.026	34	34.63	
5	1.3	1.3	2.6	0.812	24	24.45	

Calculations:

$$Qstd = 1/m[\text{Sqrt}(H2O(Pa/Pstd)(Tstd/Ta))-b]$$

$$IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$$

Qstd = standard flow rate

IC = corrected chart response

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)

Pa = actual pressure during calibration (mm Hg)

For subsequent calculation of sampler flow:

$$1/m((I)[\text{Sqrt}(298/Tav)(Pav/760)]-b)$$


m = sampler slope

b = sampler intercept

I = chart response

Tav = daily average temperature

Pav = daily average pressure

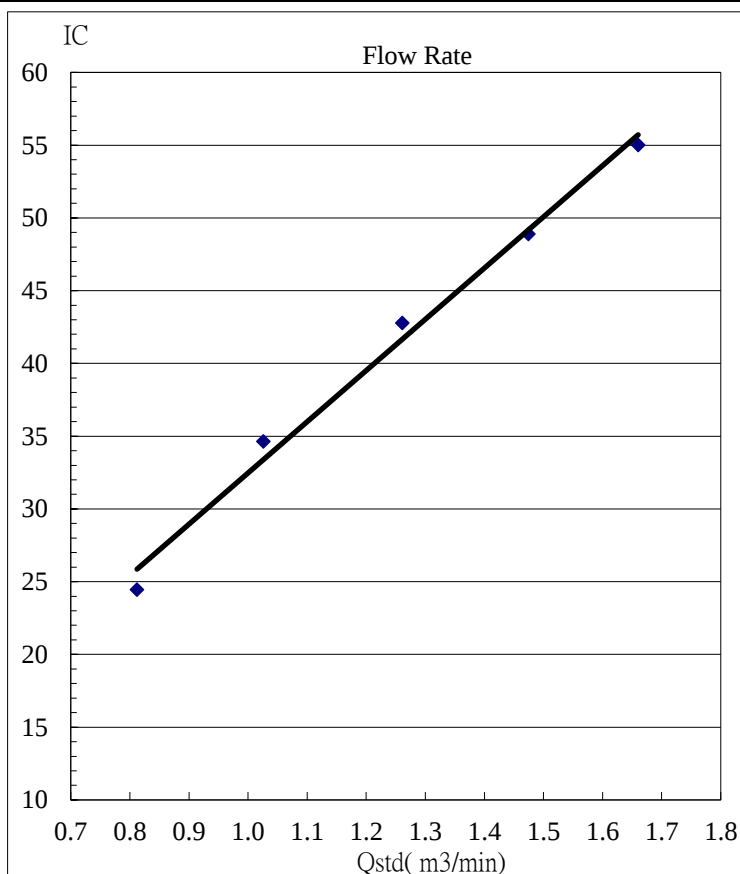

TSP SAMPLER CALIBRATION CALCULATION SPREADSHEET

Location ID: AM2	Date of Calibration:	16-Dec-24
Name and Model : TISCH HVS Model TE-5170	Next Calibration Date:	16-Feb-25
	Operator:	P.F.Yeung

CONDITIONS

Sea Level Pressure (hpa)	1022.7	Corrected Pressure (mm Hg)	767.1
Temperature (°C)	17.0	Temperature (K)	290

CALIBRATION ORIFICE

Make:	TISCH	Qstd Slope	2.08315
Model:	TE-5025A	Qstd Intercept	-0.04938
Serial#:	2454		

CALIBRATION

Plate No.	H2O(L) (in)	H2O(R) (in)	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)	LINEAR REGRESSION
18	6.2	6.2	12.4	1.746	55	56.03	Slope= 30.970 Intercept= 2.602 Corr. Coeff.= 0.9989
13	4.8	4.8	9.6	1.539	50	50.93	
10	3.7	3.7	7.4	1.354	44	44.82	
7	2.3	2.3	4.6	1.073	35	35.65	
5	1.4	1.4	2.8	0.842	28	28.52	

Calculations:

$$Qstd = 1/m[\text{Sqrt}(H2O(Pa/Pstd)(Tstd/Ta))-b]$$

$$IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$$

Qstd = standard flow rate

IC = corrected chart response

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)

Pa = actual pressure during calibration (mm Hg)

For subsequent calculation of sampler flow:

$$1/m((I)[\text{Sqrt}(298/Tav)(Pav/760)]-b)$$


m = sampler slope

b = sampler intercept

I = chart response

Tav = daily average temperature

Pav = daily average pressure

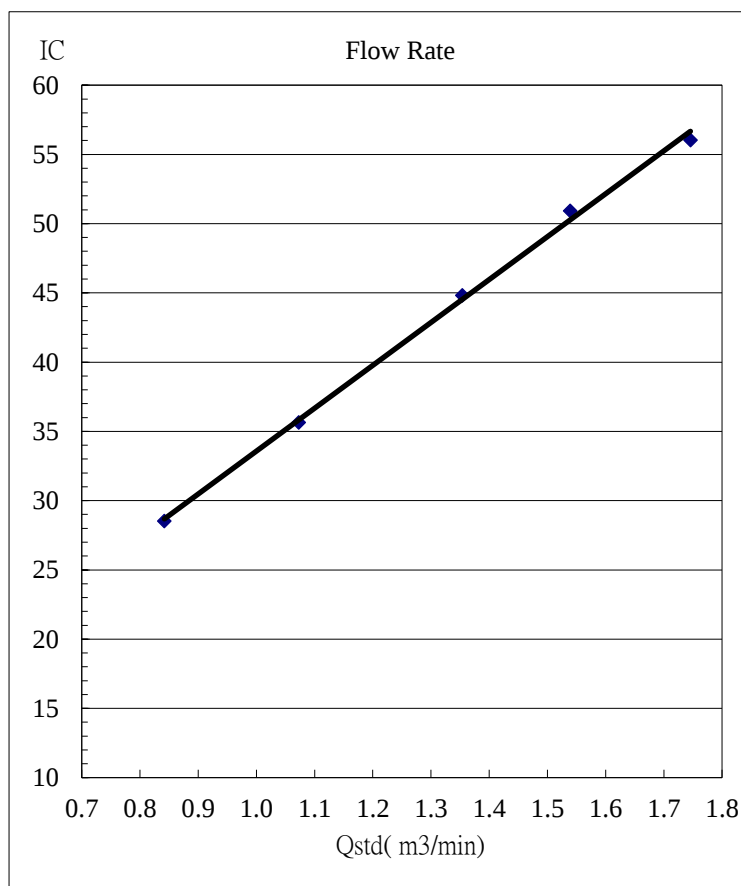

TSP SAMPLER CALIBRATION CALCULATION SPREADSHEET

Location ID: AM3	Date of Calibration:	16-Dec-24
Name and Model : TISCH HVS Model TE-5170	Next Calibration Date:	16-Feb-25
	Operator:	P.F.Yeung

CONDITIONS

Sea Level Pressure (hpa)	1022.7	Corrected Pressure (mm Hg)	767.1
Temperature (°C)	17.0	Temperature (K)	290

CALIBRATION ORIFICE

Make:	TISCH	Qstd Slope	2.08315
Model:	TE-5025A	Qstd Intercept	-0.04938
Serial#:	2454		

CALIBRATION

Plate No.	H2O(L) (in)	H2O(R) (in)	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)	LINEAR REGRESSION
18	5.8	5.9	11.7	1.696	57	58.06	Slope= 27.680 Intercept= 11.209 Corr. Coeff.= 0.9953
13	4.6	4.6	9.2	1.507	52	52.97	
10	3.5	3.4	6.9	1.308	46	46.86	
7	2.2	2.2	4.4	1.049	41	41.77	
5	1.4	1.4	2.8	0.842	33	33.62	

Calculations:

$$Qstd = 1/m[\text{Sqrt}(H2O(Pa/Pstd)(Tstd/Ta))-b]$$

$$IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$$

Qstd = standard flow rate

IC = corrected chart response

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)

Pa = actual pressure during calibration (mm Hg)

For subsequent calculation of sampler flow:

$$1/m((I)[\text{Sqrt}(298/Tav)(Pav/760)]-b)$$


m = sampler slope

b = sampler intercept

I = chart response

Tav = daily average temperature

Pav = daily average pressure

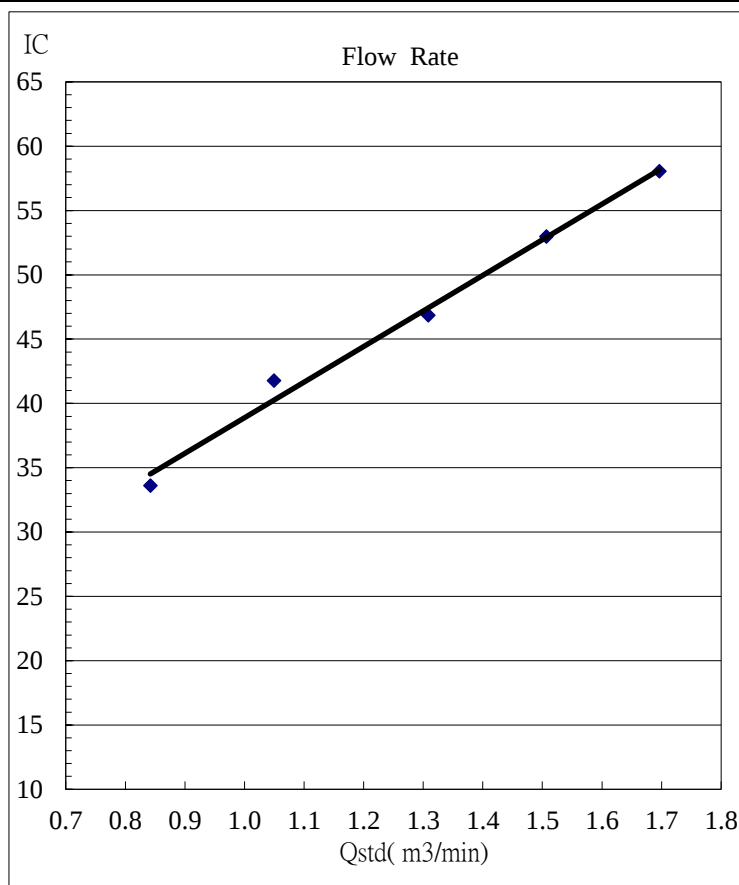

TSP SAMPLER CALIBRATION CALCULATION SPREADSHEET

Location ID: AM4	Date of Calibration:	16-Dec-24
Name and Model : TISCH HVS Model TE-5170	Next Calibration Date:	16-Feb-25
	Operator:	P.F.Yeung

CONDITIONS

Sea Level Pressure (hpa)	1022.7	Corrected Pressure (mm Hg)	767.1
Temperature (°C)	17.0	Temperature (K)	290

CALIBRATION ORIFICE

Make:	TISCH	Qstd Slope	2.08315
Model:	TE-5025A	Qstd Intercept	-0.04938
Serial#:	2454		

CALIBRATION

Plate No.	H2O(L) (in)	H2O(R) (in)	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)	LINEAR REGRESSION
18	6.3	6.2	12.5	1.753	58	59.08	Slope= 32.169 Intercept= 2.782 Corr. Coeff.= 0.9982
13	5.0	4.9	9.9	1.562	52	52.97	
10	3.7	3.6	7.3	1.345	45	45.84	
7	2.2	2.2	4.4	1.049	37	37.69	
5	1.5	1.4	2.9	0.856	29	29.54	

Calculations:

$$Qstd = 1/m[\text{Sqrt}(H2O(Pa/Pstd)(Tstd/Ta))-b]$$

$$IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$$

Qstd = standard flow rate

IC = corrected chart response

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)

Pa = actual pressure during calibration (mm Hg)

For subsequent calculation of sampler flow:

$$1/m((I) [\text{Sqrt}(298/Tav)(Pav/760)]-b)$$


m = sampler slope

b = sampler intercept

I = chart response

Tav = daily average temperature

Pav = daily average pressure

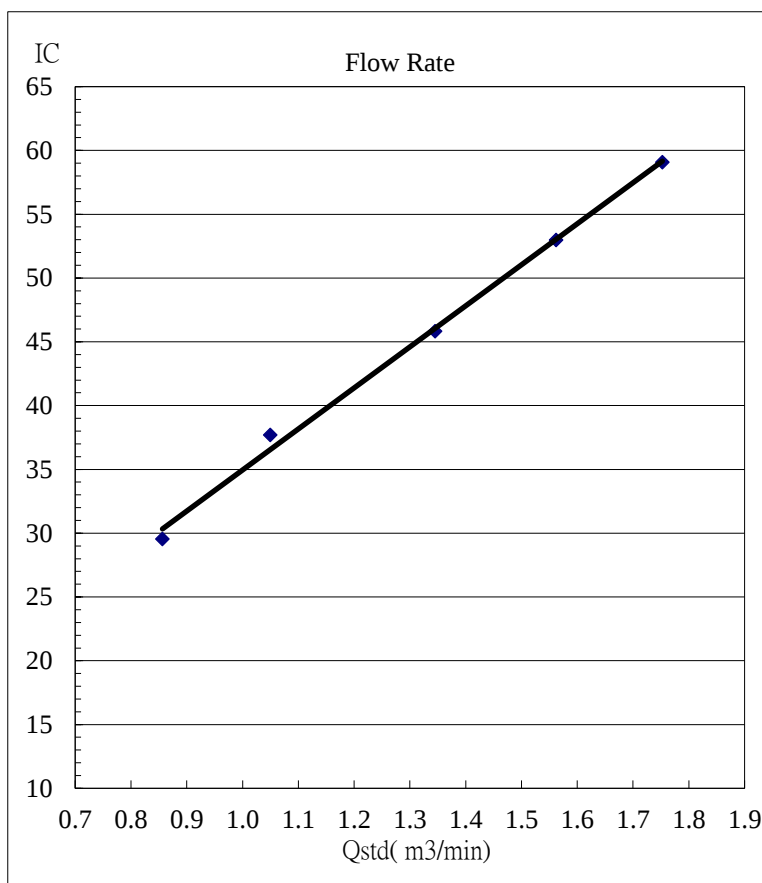

TSP SAMPLER CALIBRATION CALCULATION SPREADSHEET

Location ID: AM1	Date of Calibration:	14-Feb-25
Name and Model : TISCH HVS Model TE-5170	Next Calibration Date:	14-Apr-25
	Operator:	P.F.Yeung

CONDITIONS

	1019	Corrected Pressure (mm Hg)	764.3
Temperature (°C)	18.0	Temperature (K)	291

CALIBRATION ORIFICE

Make:	TISCH	Qstd Slope	2.08315
Model:	TE-5025A	Qstd Intercept	-0.04938
Serial#:	2454		

CALIBRATION

Plate No.	H2O(L) (in)	H2O(R) (in)	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)	LINEAR REGRESSION
18	5.6	5.6	11.2	1.654	54	54.81	Slope= 30.803 Intercept= 3.1088 Corr. Coeff.= 0.9963
13	4.7	4.7	9.4	1.518	48	48.72	
10	3.2	3.2	6.4	1.256	42	42.63	
7	2.2	2.2	4.4	1.046	34	34.51	
5	1.3	1.3	2.6	0.809	28	28.42	

Calculations:

$Qstd = 1/m[\text{Sqrt}(H2O(Pa/Pstd)(Tstd/Ta))-b]$

$IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$

Qstd = standard flow rate

IC = corrected chart response

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)

Pa = actual pressure during calibration (mm Hg)

For subsequent calculation of sampler flow:

$1/m((I)[\text{Sqrt}(298/Tav)(Pav/760)]-b)$


m = sampler slope

b = sampler intercept

I = chart response

Tav = daily average temperature

Pav = daily average pressure

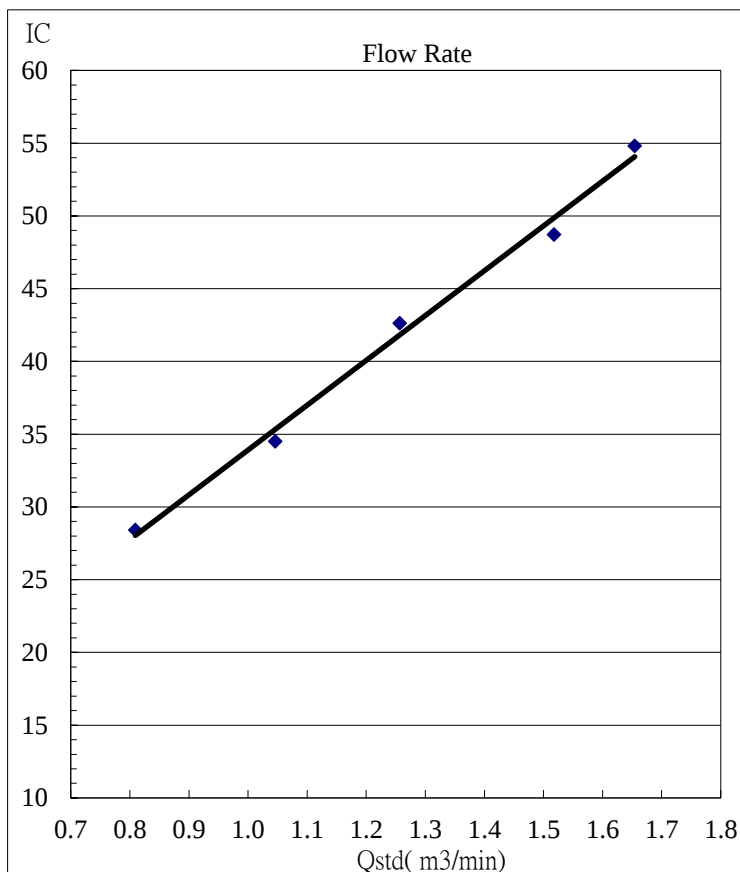

TSP SAMPLER CALIBRATION CALCULATION SPREADSHEET

Location ID: AM2	Date of Calibration:	14-Feb-25
Name and Model : TISCH HVS Model TE-5170	Next Calibration Date:	14-Apr-25
	Operator:	P.F.Yeung

CONDITIONS

Sea Level Pressure (hpa)	1019	Corrected Pressure (mm Hg)	764.3
Temperature (°C)	18.0	Temperature (K)	291

CALIBRATION ORIFICE

Make:	TISCH	Qstd Slope	2.08315
Model:	TE-5025A	Qstd Intercept	-0.04938
Serial#:	2454		

CALIBRATION

Plate No.	H2O(L) (in)	H2O(R) (in)	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)	LINEAR REGRESSION
18	6.6	6.6	13.2	1.794	53	53.80	Slope= 28.312 Intercept= 3.469 Corr. Coeff.= 0.9987
13	5.2	5.2	10.4	1.595	48	48.72	
10	3.8	3.8	7.6	1.367	42	42.63	
7	2.5	2.5	5.0	1.113	35	35.53	
5	1.5	1.5	3.0	0.868	27	27.41	

Calculations:

$$Qstd = 1/m[\text{Sqrt}(H2O(Pa/Pstd)(Tstd/Ta))-b]$$

$$IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$$

Qstd = standard flow rate

IC = corrected chart response

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)

Pa = actual pressure during calibration (mm Hg)

For subsequent calculation of sampler flow:

$$1/m((I) [\text{Sqrt}(298/Tav)(Pav/760)]-b)$$


m = sampler slope

b = sampler intercept

I = chart response

Tav = daily average temperature

Pav = daily average pressure

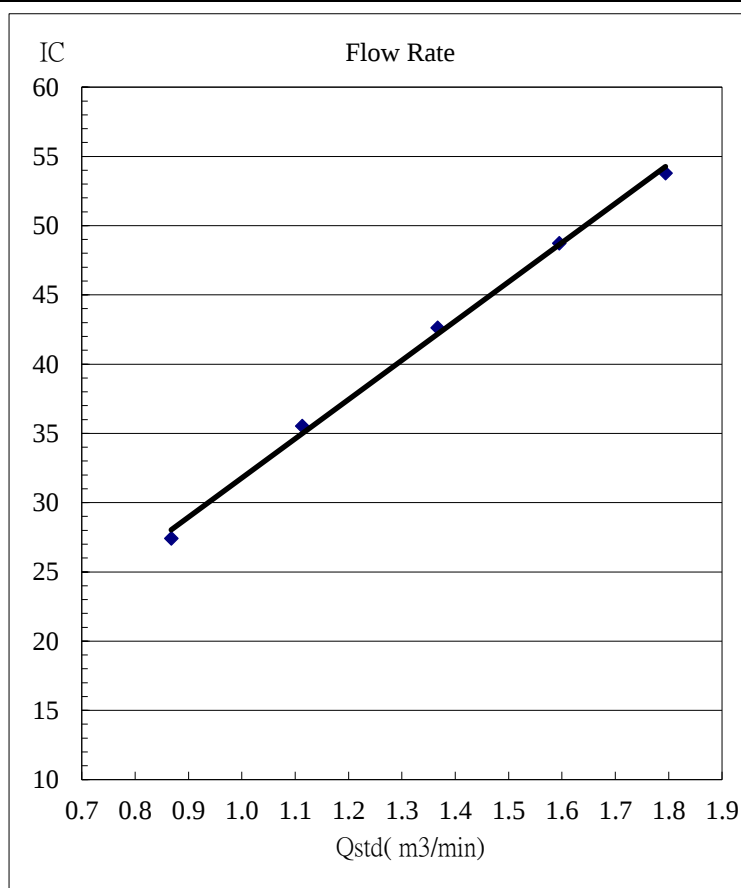

TSP SAMPLER CALIBRATION CALCULATION SPREADSHEET

Location ID: AM3	Date of Calibration:	14-Feb-25
Name and Model : TISCH HVS Model TE-5170	Next Calibration Date:	14-Apr-25
	Operator:	P.F.Yeung

CONDITIONS

Sea Level Pressure (hpa)	1019	Corrected Pressure (mm Hg)	764.3
Temperature (°C)	18.0	Temperature (K)	291

CALIBRATION ORIFICE

Make:	TISCH	Qstd Slope	2.08315
Model:	TE-5025A	Qstd Intercept	-0.04938
Serial#:	2454		

CALIBRATION

Plate No.	H2O(L) (in)	H2O(R) (in)	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)	LINEAR REGRESSION
18	5.9	5.9	11.8	1.698	58	58.87	Slope= 26.234 Intercept= 14.767 Corr. Coeff.= 0.9941
13	4.6	4.6	9.2	1.502	53	53.80	
10	3.2	3.2	6.4	1.256	48	48.72	
7	2.1	2.1	4.2	1.022	42	42.63	
5	1.4	1.4	2.8	0.839	35	35.53	

Calculations:

$$Qstd = 1/m[\text{Sqrt}(H2O(Pa/Pstd)(Tstd/Ta))-b]$$

$$IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$$

Qstd = standard flow rate

IC = corrected chart response

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)

Pa = actual pressure during calibration (mm Hg)

For subsequent calculation of sampler flow:

$$1/m((I) [\text{Sqrt}(298/Tav)(Pav/760)]-b)$$


m = sampler slope

b = sampler intercept

I = chart response

Tav = daily average temperature

Pav = daily average pressure

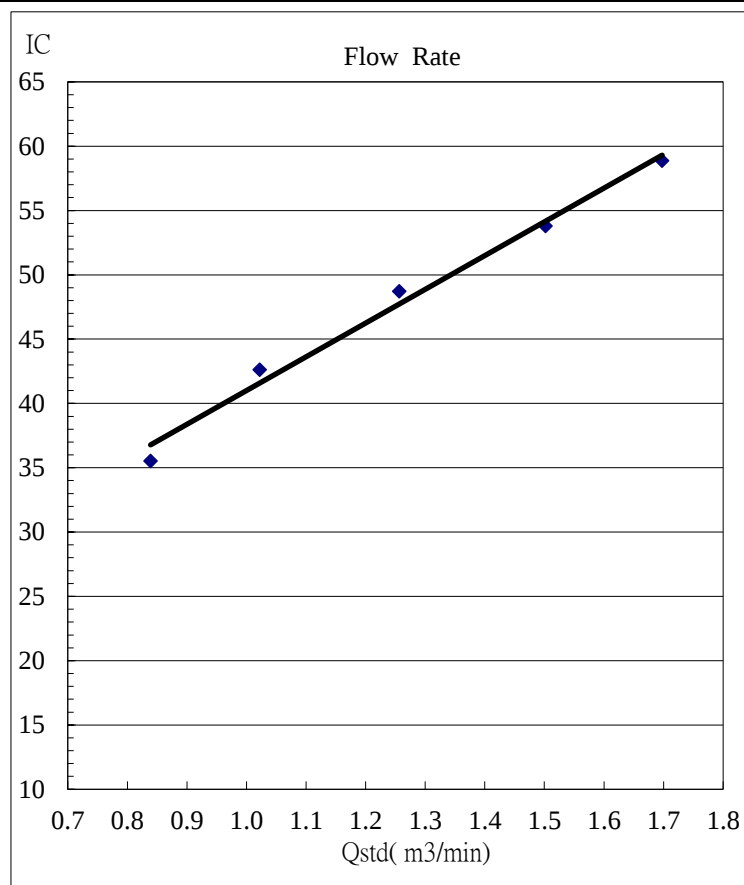

TSP SAMPLER CALIBRATION CALCULATION SPREADSHEET

Location ID: AM4	Date of Calibration:	14-Feb-25
Name and Model : TISCH HVS Model TE-5170	Next Calibration Date:	14-Apr-25
	Operator:	P.F.Yeung

CONDITIONS

Sea Level Pressure (hpa)	1019	Corrected Pressure (mm Hg)	764.3
Temperature (°C)	18.0	Temperature (K)	291

CALIBRATION ORIFICE

Make:	TISCH	Qstd Slope	2.08315
Model:	TE-5025A	Qstd Intercept	-0.04938
Serial#:	2454		

CALIBRATION

Plate No.	H2O(L) (in)	H2O(R) (in)	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)	LINEAR REGRESSION
18	6.5	6.5	13.0	1.781	57	57.86	Slope= 30.302 Intercept= 3.414 Corr. Coeff.= 0.9984
13	5.2	5.2	10.4	1.595	51	51.77	
10	3.7	3.7	7.4	1.349	43	43.65	
7	2.5	2.5	5.0	1.113	36	36.54	
5	1.5	1.5	3.0	0.868	30	30.45	

Calculations:

$$Qstd = 1/m[\text{Sqrt}(H2O(Pa/Pstd)(Tstd/Ta))-b]$$

$$IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$$

Qstd = standard flow rate

IC = corrected chart response

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)

Pa = actual pressure during calibration (mm Hg)

For subsequent calculation of sampler flow:

$$1/m((I)[\text{Sqrt}(298/Tav)(Pav/760)]-b)$$

m = sampler slope

b = sampler intercept

I = chart response

Tav = daily average temperature

Pav = daily average pressure

