



ANNEX D1

CALIBRATION CERTIFICATES FOR DUST
MONITORING EQUIPMENT

TSP SAMPLER CALIBRATION CALCULATION SPREADSHEET

Location ID: AM1	Date of Calibration:	9-Jun-25
Name and Model : TISCH HVS Model TE-5170	Next Calibration Date:	9-Aug-25
	Operator:	P.F.Yeung

CONDITIONS

Temperature (°C)	1004	Corrected Pressure (mm Hg)	753.1
	32.7		305.7

CALIBRATION ORIFICE

Make:	TISCH	Qstd Slope	2.08315
Model:	TE-5025A	Qstd Intercept	-0.04938
Serial#:	2454		

CALIBRATION

Plate No.	H2O(L) (in)	H2O(R) (in)	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)	LINEAR REGRESSION
18	4.9	4.9	9.8	1.501	52	51.12	Slope= 31.180 Intercept= 3.8458 Corr. Coeff.= 0.9951
13	3.9	3.9	7.8	1.342	46	45.22	
10	2.9	2.9	5.8	1.160	40	39.32	
7	1.6	1.6	3.2	0.868	33	32.44	
5	1.1	1.1	2.2	0.724	26	25.56	

Calculations:

$$Qstd = 1/m[\text{Sqrt}(H2O(Pa/Pstd)(Tstd/Ta))-b]$$

$$IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$$

Qstd = standard flow rate

IC = corrected chart response

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)

Pa = actual pressure during calibration (mm Hg)

For subsequent calculation of sampler flow:

$$1/m((I)[\text{Sqrt}(298/Tav)(Pav/760)]-b)$$


m = sampler slope

b = sampler intercept

I = chart response

Tav = daily average temperature

Pav = daily average pressure

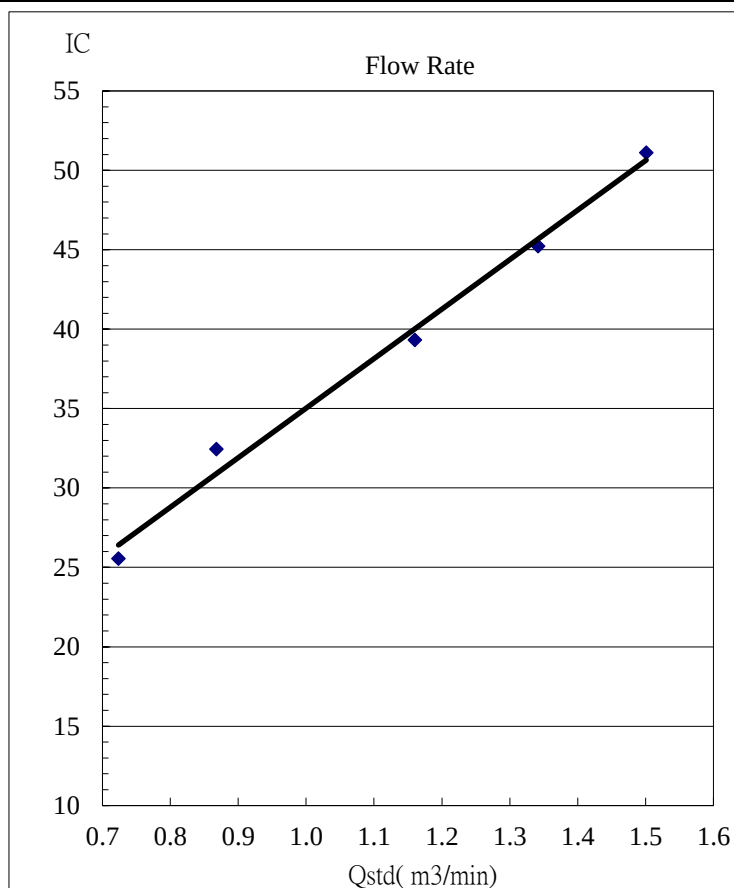

TSP SAMPLER CALIBRATION CALCULATION SPREADSHEET

Location ID: AM2	Date of Calibration:	9-Jun-25
Name and Model : TISCH HVS Model TE-5170	Next Calibration Date:	9-Aug-25
	Operator:	P.F.Yeung

CONDITIONS

Sea Level Pressure (hpa)	1004	Corrected Pressure (mm Hg)	753.1
Temperature (°C)	32.7	Temperature (K)	305.7

CALIBRATION ORIFICE

Make:	TISCH	Qstd Slope	2.08315
Model:	TE-5025A	Qstd Intercept	-0.04938
Serial#:	2454		

CALIBRATION

Plate No.	H2O(L) (in)	H2O(R) (in)	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)	LINEAR REGRESSION
18	6.0	6.0	12.0	1.658	54	53.09	Slope= 29.964 Intercept= 4.0069 Corr. Coeff.= 0.9982
13	4.6	4.6	9.2	1.455	49	48.17	
10	3.4	3.4	6.8	1.254	43	42.27	
7	2.3	2.3	4.6	1.036	35	34.41	
5	1.3	1.3	2.6	0.785	28	27.53	

Calculations:

$$Qstd = 1/m[\text{Sqrt}(H2O(Pa/Pstd)(Tstd/Ta))-b]$$

$$IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$$

Qstd = standard flow rate

IC = corrected chart response

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)

Pa = actual pressure during calibration (mm Hg)

For subsequent calculation of sampler flow:

$$1/m((I)[\text{Sqrt}(298/Tav)(Pav/760)]-b)$$


m = sampler slope

b = sampler intercept

I = chart response

Tav = daily average temperature

Pav = daily average pressure

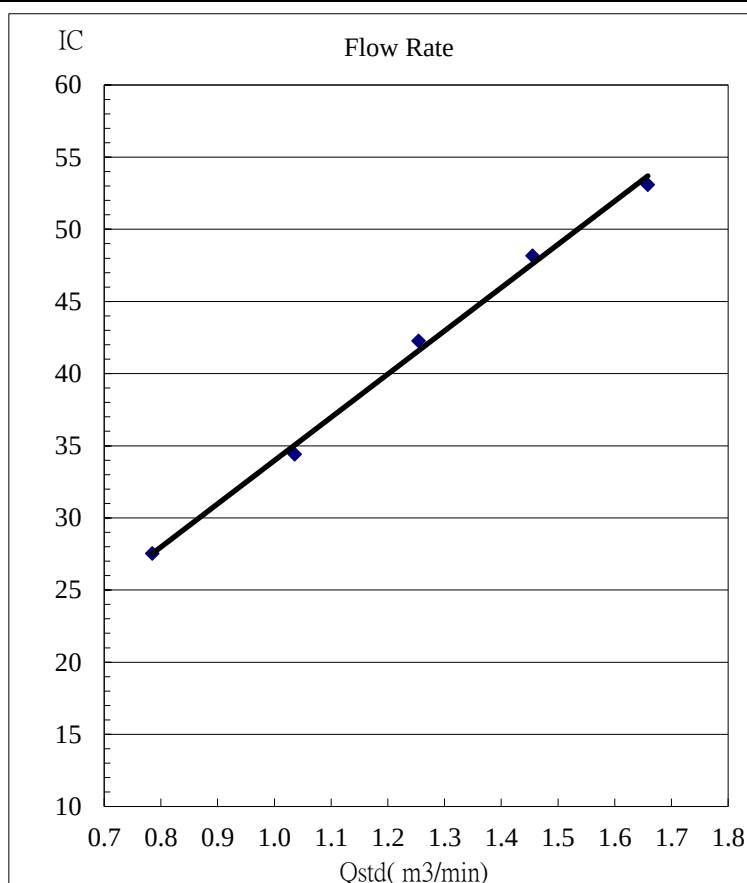

TSP SAMPLER CALIBRATION CALCULATION SPREADSHEET

Location ID: AM3	Date of Calibration:	9-Jun-25
Name and Model : TISCH HVS Model TE-5170	Next Calibration Date:	9-Aug-25
	Operator:	P.F.Yeung

CONDITIONS

Sea Level Pressure (hpa)	1004	Corrected Pressure (mm Hg)	753.1
Temperature (°C)	32.7	Temperature (K)	305.7

CALIBRATION ORIFICE

Make:	TISCH	Qstd Slope	2.08315
Model:	TE-5025A	Qstd Intercept	-0.04938
Serial#:	2454		

CALIBRATION

Plate No.	H2O(L) (in)	H2O(R) (in)	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)	LINEAR REGRESSION
18	5.3	5.3	10.6	1.560	56	55.05	Slope= 28.897 Intercept= 9.6135 Corr. Coeff.= 0.9946
13	4.3	4.3	8.6	1.408	50	49.15	
10	3.0	3.0	6.0	1.180	45	44.24	
7	2.1	2.1	4.2	0.991	40	39.32	
5	1.3	1.3	2.6	0.785	32	31.46	

Calculations:

$$Qstd = 1/m[\text{Sqrt}(H2O(Pa/Pstd)(Tstd/Ta))-b]$$

$$IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$$

Qstd = standard flow rate

IC = corrected chart response

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)

Pa = actual pressure during calibration (mm Hg)

For subsequent calculation of sampler flow:

$$1/m((I)[\text{Sqrt}(298/Tav)(Pav/760)]-b)$$


m = sampler slope

b = sampler intercept

I = chart response

Tav = daily average temperature

Pav = daily average pressure

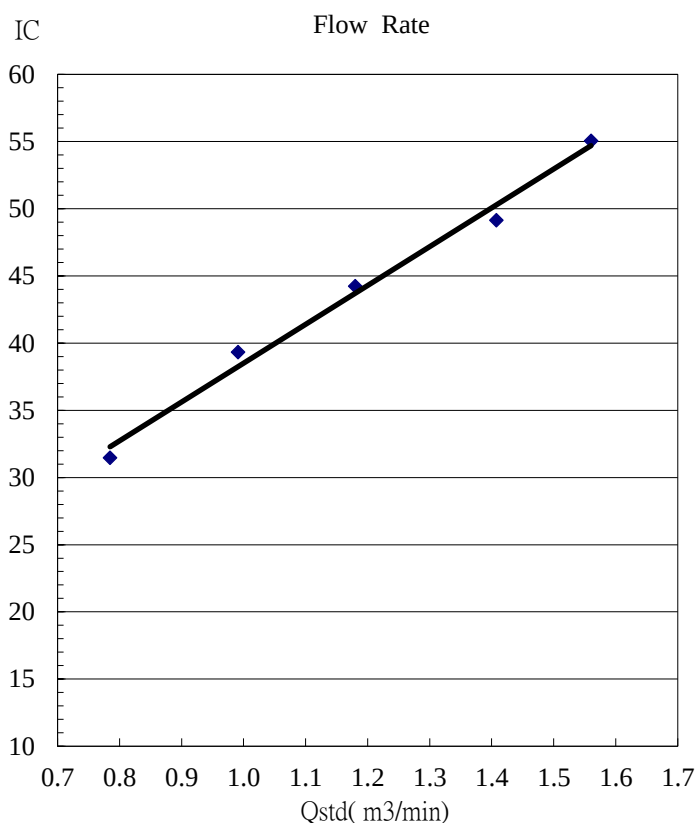

TSP SAMPLER CALIBRATION CALCULATION SPREADSHEET

Location ID: AM4	Date of Calibration:	9-Jun-25
Name and Model : TISCH HVS Model TE-5170	Next Calibration Date:	9-Aug-25
	Operator:	P.F.Yeung

CONDITIONS

Sea Level Pressure (hpa)	1004	Corrected Pressure (mm Hg)	753.1
Temperature (°C)	32.7	Temperature (K)	305.7

CALIBRATION ORIFICE

Make:	TISCH	Qstd Slope	2.08315
Model:	TE-5025A	Qstd Intercept	-0.04938
Serial#:	2454		

CALIBRATION

Plate No.	H2O(L) (in)	H2O(R) (in)	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)	LINEAR REGRESSION
18	5.9	5.9	11.8	1.645	55	54.07	Slope= 31.445 Intercept= 3.3216 Corr. Coeff.= 0.9966
13	4.5	4.5	9.0	1.439	50	49.15	
10	3.4	3.3	6.7	1.245	44	43.25	
7	2.2	2.1	4.3	1.002	36	35.39	
5	1.4	1.3	2.7	0.799	28	27.53	

Calculations:

$$Qstd = 1/m[\text{Sqrt}(H2O(Pa/Pstd)(Tstd/Ta))-b]$$

$$IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$$

Qstd = standard flow rate

IC = corrected chart response

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)

Pa = actual pressure during calibration (mm Hg)

For subsequent calculation of sampler flow:

$$1/m((I) [\text{Sqrt}(298/Tav)(Pav/760)]-b)$$


m = sampler slope

b = sampler intercept

I = chart response

Tav = daily average temperature

Pav = daily average pressure

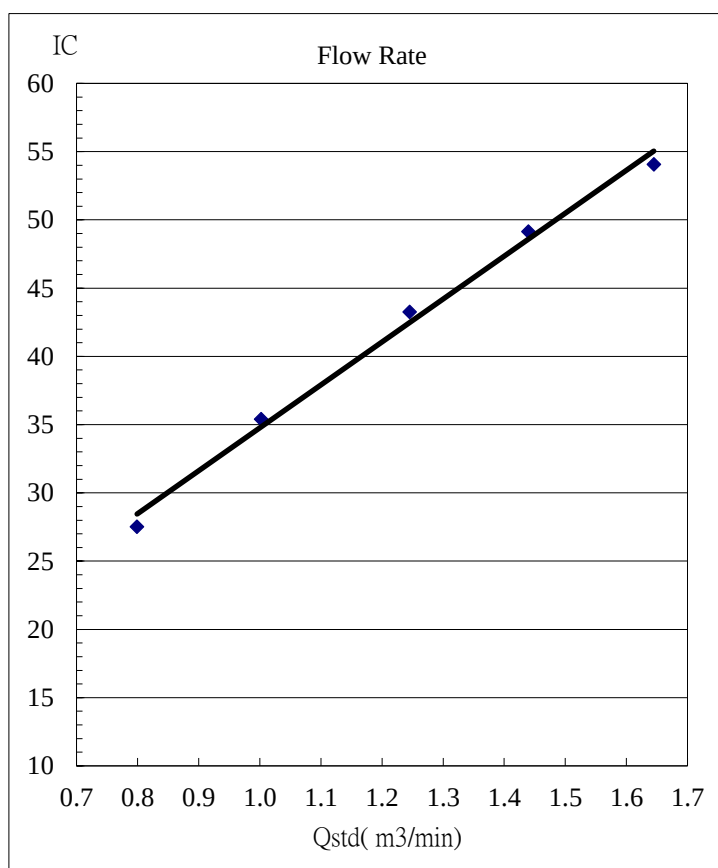

TSP SAMPLER CALIBRATION CALCULATION SPREADSHEET

Location ID: AM1	Date of Calibration:	9-Aug-25
Name and Model : TISCH HVS Model TE-5170	Next Calibration Date:	9-Oct-25
	Operator:	P.F.Yeung

CONDITIONS

	1015	Corrected Pressure (mm Hg)	757.9
Temperature (°C)	33.0	Temperature (K)	306.0

CALIBRATION ORIFICE

Make:	TISCH	Qstd Slope	2.08315
Model:	TE-5025A	Qstd Intercept	-0.04938
Serial#:	2454		

CALIBRATION

Plate No.	H2O(L) (in)	H2O(R) (in)	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)	LINEAR REGRESSION
18	4.9	4.9	9.8	1.505	51	50.26	Slope= 32.779 Intercept= 1.301 Corr. Coeff.= 0.9991
13	3.9	3.9	7.8	1.345	46	45.33	
10	2.8	2.8	5.6	1.143	40	39.42	
7	1.9	1.9	3.8	0.946	33	32.52	
5	1.1	1.1	2.2	0.725	25	24.64	

Calculations:

$$Qstd = 1/m[\text{Sqrt}(H2O(Pa/Pstd)(Tstd/Ta))-b]$$

$$IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$$

Qstd = standard flow rate

IC = corrected chart response

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)

Pa = actual pressure during calibration (mm Hg)

For subsequent calculation of sampler flow:

$$1/m((I)[\text{Sqrt}(298/Tav)(Pav/760)]-b)$$


m = sampler slope

b = sampler intercept

I = chart response

Tav = daily average temperature

Pav = daily average pressure

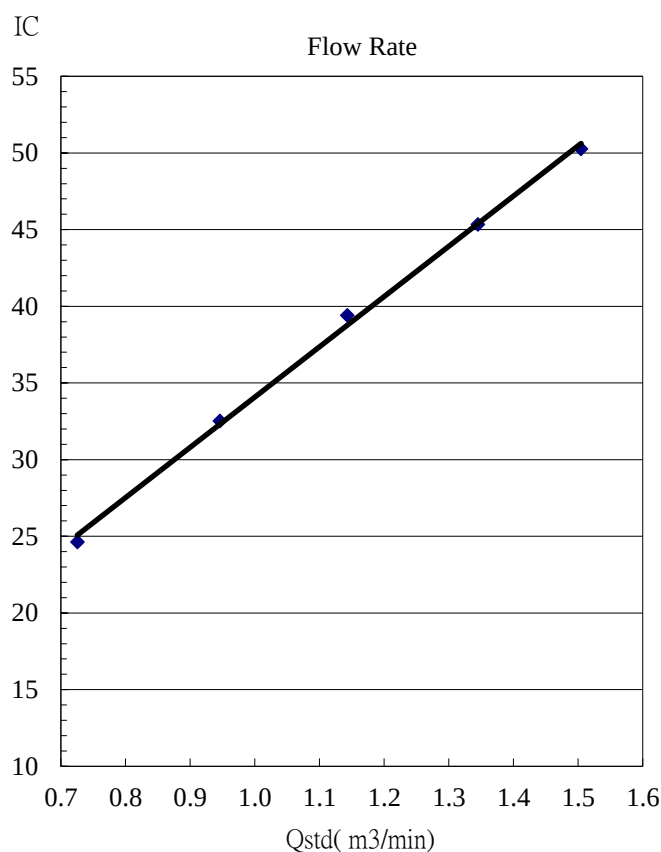

TSP SAMPLER CALIBRATION CALCULATION SPREADSHEET

Location ID: AM2	Date of Calibration:	9-Aug-25
Name and Model : TISCH HVS Model TE-5170	Next Calibration Date:	9-Oct-25
	Operator:	P.F.Yeung

CONDITIONS

Sea Level Pressure (hpa)	1010	Corrected Pressure (mm Hg)	757.9
Temperature (°C)	33.0	Temperature (K)	306.0

CALIBRATION ORIFICE

Make:	TISCH	Qstd Slope	2.08315
Model:	TE-5025A	Qstd Intercept	-0.04938
Serial#:	2454		

CALIBRATION

Plate No.	H2O(L) (in)	H2O(R) (in)	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)	LINEAR REGRESSION
18	5.8	5.8	11.6	1.635	53	52.23	Slope= 28.796 Intercept= 5.766 Corr. Coeff.= 0.9954
13	4.3	4.3	8.6	1.411	48	47.30	
10	3.4	3.4	6.8	1.257	42	41.39	
7	2.1	2.1	4.2	0.993	36	35.48	
5	1.3	1.3	2.6	0.787	28	27.59	

Calculations:

$$Qstd = 1/m[\text{Sqrt}(H2O(Pa/Pstd)(Tstd/Ta))-b]$$

$$IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$$

Qstd = standard flow rate

IC = corrected chart response

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)

Pa = actual pressure during calibration (mm Hg)

For subsequent calculation of sampler flow:

$$1/m((I) [\text{Sqrt}(298/Tav)(Pav/760)]-b)$$


m = sampler slope

b = sampler intercept

I = chart response

Tav = daily average temperature

Pav = daily average pressure

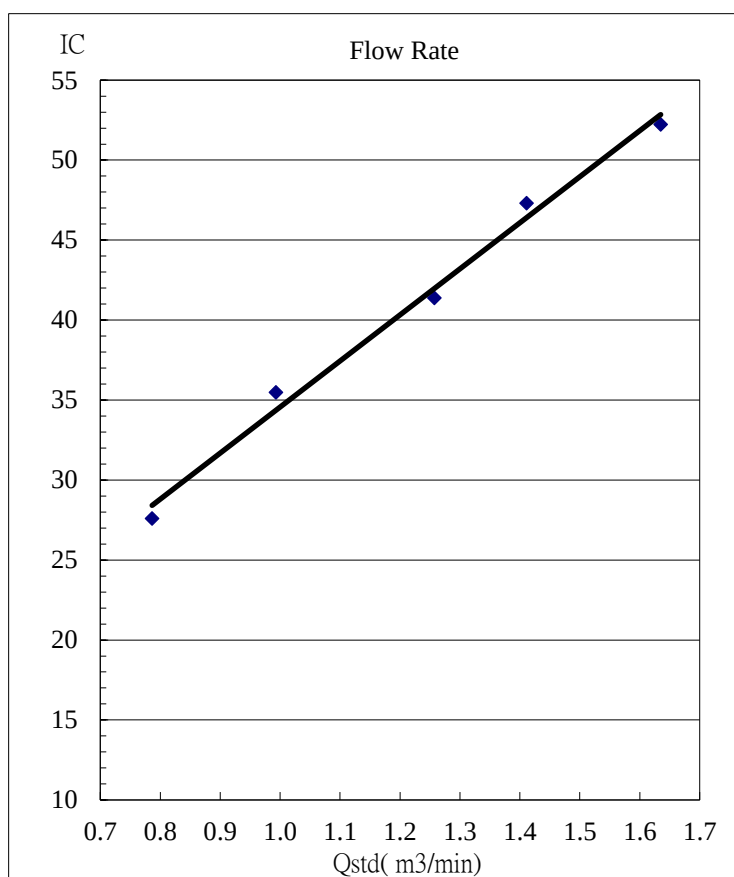

TSP SAMPLER CALIBRATION CALCULATION SPREADSHEET

Location ID: AM3	Date of Calibration:	9-Aug-25
Name and Model : TISCH HVS Model TE-5170	Next Calibration Date:	9-Oct-25
	Operator:	P.F.Yeung

CONDITIONS

Sea Level Pressure (hpa)	1010	Corrected Pressure (mm Hg)	757.9
Temperature (°C)	33.0	Temperature (K)	306.0

CALIBRATION ORIFICE

Make:	TISCH	Qstd Slope	2.08315
Model:	TE-5025A	Qstd Intercept	-0.04938
Serial#:	2454		

CALIBRATION

Plate No.	H2O(L) (in)	H2O(R) (in)	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)	LINEAR REGRESSION
18	5.4	5.4	10.8	1.578	56	55.19	Slope= 28.490 Intercept= 9.840 Corr. Coeff.= 0.9908
13	4.5	4.5	9.0	1.443	51	50.26	
10	3.2	3.2	6.4	1.221	45	44.35	
7	2.1	2.1	4.2	0.993	40	39.42	
5	1.3	1.3	2.6	0.787	32	31.54	

Calculations:

$$Qstd = 1/m[\text{Sqrt}(H2O(Pa/Pstd)(Tstd/Ta))-b]$$

$$IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$$

Qstd = standard flow rate

IC = corrected chart response

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)

Pa = actual pressure during calibration (mm Hg)

For subsequent calculation of sampler flow:

$$1/m((I) [\text{Sqrt}(298/Tav)(Pav/760)]-b)$$


m = sampler slope

b = sampler intercept

I = chart response

Tav = daily average temperature

Pav = daily average pressure

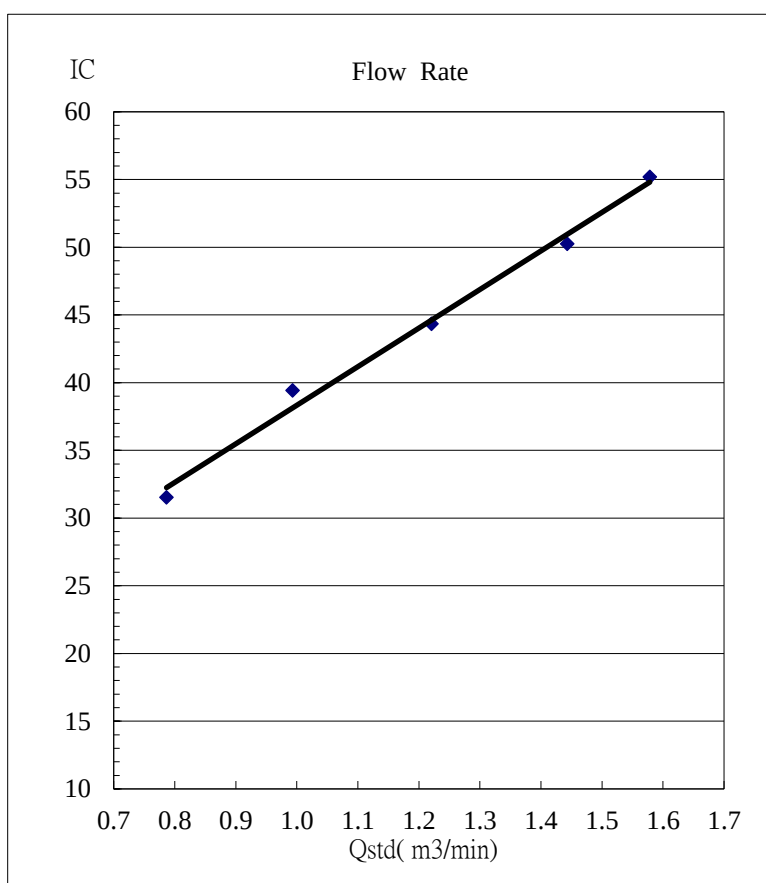

TSP SAMPLER CALIBRATION CALCULATION SPREADSHEET

Location ID: AM4	Date of Calibration:	9-Aug-25
Name and Model : TISCH HVS Model TE-5170	Next Calibration Date:	9-Oct-25
	Operator:	P.F.Yeung

CONDITIONS

Sea Level Pressure (hpa)	1010	Corrected Pressure (mm Hg)	757.9
Temperature (°C)	33.0	Temperature (K)	306.0

CALIBRATION ORIFICE

Make:	TISCH	Qstd Slope	2.08315
Model:	TE-5025A	Qstd Intercept	-0.04938
Serial#:	2454		

CALIBRATION

Plate No.	H2O(L) (in)	H2O(R) (in)	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)	LINEAR REGRESSION
18	5.6	5.6	11.2	1.607	56	55.19	Slope= 29.982 Intercept= 7.137 Corr. Coeff.= 0.9992
13	4.4	4.4	8.8	1.427	51	50.26	
10	3.4	3.4	6.8	1.257	45	44.35	
7	2.1	2.1	4.2	0.993	38	37.45	
5	1.2	1.2	2.4	0.757	30	29.57	

Calculations:

$$Qstd = 1/m[\text{Sqrt}(H2O(Pa/Pstd)(Tstd/Ta))-b]$$

$$IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$$

Qstd = standard flow rate

IC = corrected chart response

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)

Pa = actual pressure during calibration (mm Hg)

For subsequent calculation of sampler flow:

$$1/m((I[\text{Sqrt}(298/Tav)(Pav/760)]-b)$$

m = sampler slope

b = sampler intercept

I = chart response

Tav = daily average temperature

Pav = daily average pressure

